




welch



# GC Consumables

Quality, Innovation, Competitive Price



Welch Materials is a multinational company that develops and manufactures chromatography consumables including analytical and preparative HPLC columns, Solid Phase Extraction (SPE) columns, GC columns, bulk packing materials, and protein purification products.

Welch Materials was established in 2003 at Shanghai, China and Welch Materials (Zhejiang) was opened in 2011 at Jinhua, Zhejiang, China. Welch has established operations at Welch Materials, Inc., at West Haven, CT, USA and Welch Materials, India Pvt. Ltd., at Gurgaon.

Welch strength lies in our deep experience in particle surface modification science. We are experts in bonding chemistry and innovative packing materials for chromatography applications. Utilizing and optimizing our resources, we have developed many innovative products including five series of HPLC columns including Ultisil®, Welchrom®, Xtimate®, Topsil®, and Boltimate™ and market and support these products on worldwide basis.



# Content

## Outline of GC Column

|     |                                      |    |
|-----|--------------------------------------|----|
| 1.1 | WM Series High Performance GC Column | 2  |
| 1.2 | WEL Series Economical GC Column      | 13 |
| 1.3 | Dedicated Capillary Column           | 17 |
| 1.4 | GC Packed Column                     | 20 |

## Application of GC Column

|     |                                       |    |
|-----|---------------------------------------|----|
| 2.1 | Application in Chemical Energy Field  | 22 |
| 2.2 | Application in Brewing Field          | 23 |
| 2.3 | Application in Environmental Analysis | 24 |
| 2.4 | Application in Food                   | 26 |
| 2.5 | Applications in Pharmacopoeia         | 28 |
| 2.6 | Application in Other Aspects          | 32 |

## GC Accessories

|       |                       |    |
|-------|-----------------------|----|
| 3.1   | Gas Generator         | 38 |
| 3.2   | Gas Phase Accessories | 38 |
| 3.2.1 | Injection Septa       | 38 |
| 3.2.2 | Graphite Ferrule      | 40 |
| 3.2.3 | Ordering Information  | 40 |

## Solutions for Pesticide Residue Detection

## Technical Reference

|     |                            |    |
|-----|----------------------------|----|
| 5.1 | Selection of GC Columns    | 48 |
| 5.2 | Installation of GC Columns | 49 |
| 5.3 | GC Column Troubleshooting  | 51 |

## Outline of GC Column

Welch Materials have concentrated on GC R&D and production for many years, and each column would be tested strictly before selling with attached column report. Welch columns are characterized by stable properties, high column efficiency and good reproducibility. Welch Gas column can be divided into two types: WM Series High Performance GC Column and WEL Series Economical GC Column, which can meet the analysis requirements of various customers.

Welch also provides services as sample analysis, method development, column recommendation, after-sales support and training for customers.


With good product performance and perfect after-sales service system, our GC columns have been widely used in universities, research institutes, pharmaceutical, petrochemical, brewing, environmental protection or other industries.

### 1.1 WM Series High Performance GC Column



WM series of capillary columns adopt strict technique and performance detection with strength in super inertness, low loss, high column efficiency, high selectivity, stable reproducibility and long lifetime.

#### (1) Super Inertness and Low Loss GC/MS Column

- ▶ The unique surface deactivating technique ensures the super high inertness of column, and the peak type of separation component is sharp and symmetrical.
- ▶ Bonding and cross-linking technology allow the column to keep a low loss level at higher temperature with good stability and long lifetime.

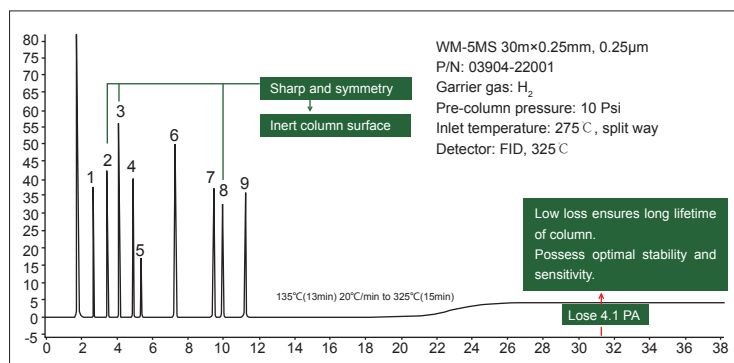

#### (2) Exceptional lot-to-lot reproducibility

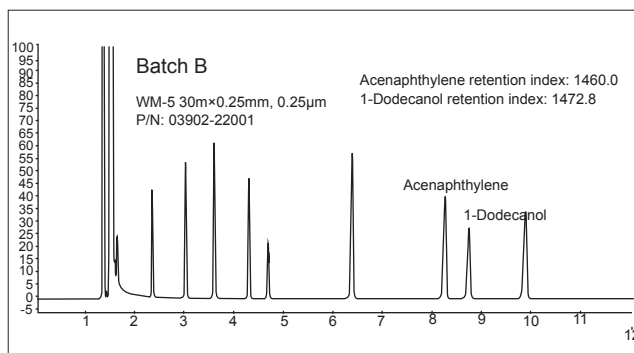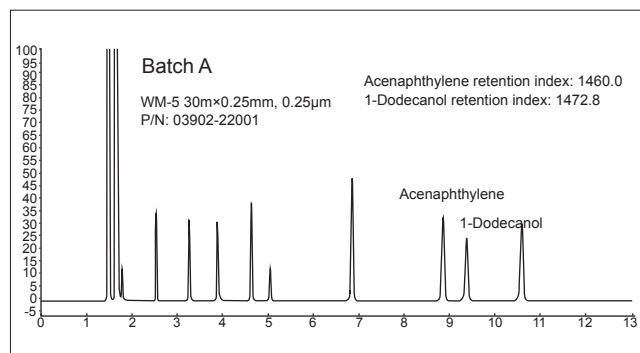


- ▶ The consistency of column inertness and superior inter-column reproducibility can be guaranteed by mixed standards samples test.
- ▶ Higher detection sensitivity and more accurate analysis results.


#### Case of Excellent Performance of WM Column

Determination of 37 fatty acids

Welch has released 37 fatty acid dedicated columns with excellent separation performance and reproducibility. Benefited from the optimized method, the analysis time can be greatly shortened without losing the resolution and the customer's analysis cost can be saved.

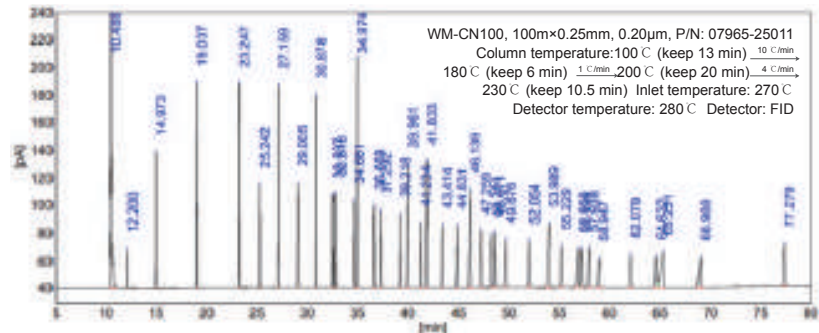


## Method Optimization

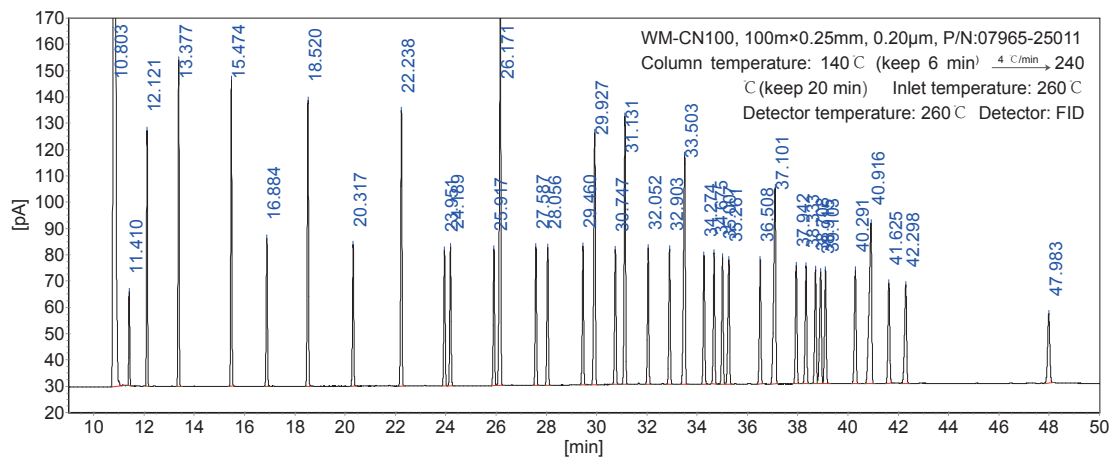

## Determination of 22 Kinds of Organochlorine Pesticide Residues


Welch provides an overall solution for the determination of 22 kinds of organochlorine pesticide residues, including sample pretreatment, chromatographic analysis, a complete set of products and technical support. The corresponding chromatographic analysis column and verification column are ideal substitution for named columns of the same specification.

| P/N         | Specification            | Note                |
|-------------|--------------------------|---------------------|
| 03916-22001 | WM-17 30m×0.25mm, 0.25µm | Analysis column     |
| 03901-22001 | WM-1 30m×0.25mm, 0.25µm  | Verificaiton column |

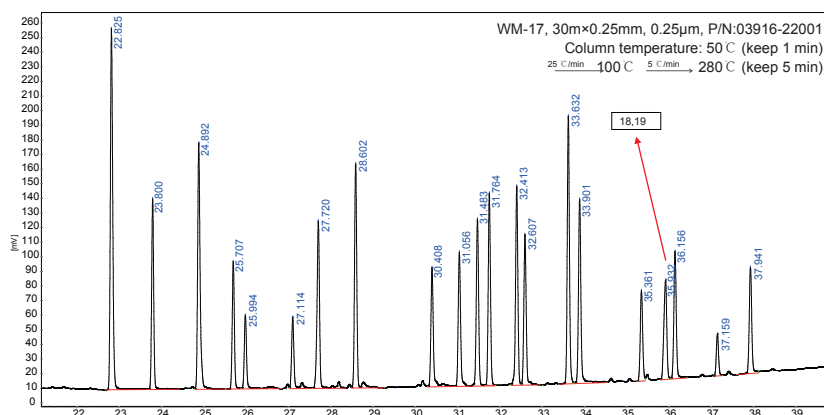





| No. | Component                | No. | Component          |
|-----|--------------------------|-----|--------------------|
| 1   | Hexachlorobenzene        | 12  | Trans-chlordane    |
| 2   | α- benzene hexachloride  | 13  | Cis-chlordane      |
| 3   | Quintozene               | 14  | α-endosulfan       |
| 4   | γ- benzene hexachloride  | 15  | p,p'-DDE           |
| 5   | β- benzene hexachloride  | 16  | Dieldrin           |
| 6   | Heptachlor               | 17  | Endrin             |
| 7   | δ- benzene hexachloride  | 18  | o,p'-DDT+ p,p'-DDD |
| 8   | Aldrin                   | 19  | o,p'-DDT+ p,p'-DDD |
| 9   | Oxychlordane             | 20  | β-endosulfan       |
| 10  | Heptachlor epoxide       | 21  | p,p'-DDT           |
| 11  | Trans-heptachlor epoxide | 22  | Endosulfan sulfate |



(Names of components in chromatogram are inferred according to files and experience)

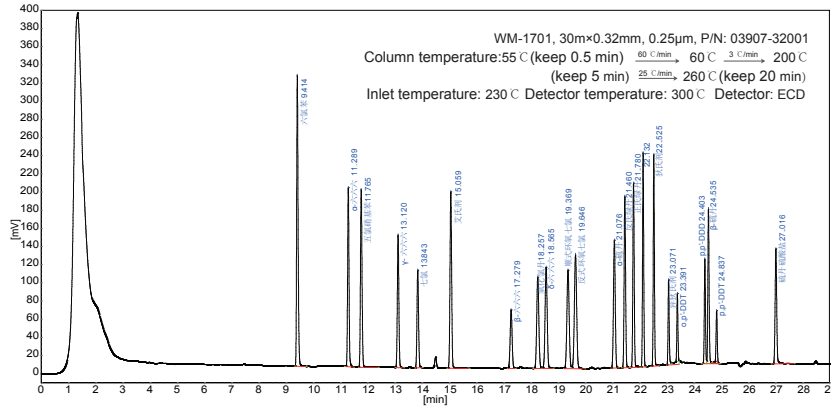

| No. | Component                | No. | Component           |
|-----|--------------------------|-----|---------------------|
| 1   | Hexachlorobenzene        | 12  | Trans-chlordane     |
| 2   | α-benzene hexachloride   | 13  | Cis-chlordane       |
| 3   | Quintozene               | 14  | α-endosulfan        |
| 4   | γ-benzene hexachloride   | 15  | p,p'-DDE            |
| 5   | β-benzene hexachloride   | 16  | Dieldrin            |
| 6   | Heptachlor               | 17  | Endrin              |
| 7   | δ-benzene hexachloride   | 18  | o,p'-DDT + p,p'-DDD |
| 8   | Aldrin                   | 19  | β-endosulfan        |
| 9   | Oxychlorane              | 20  | p,p'-DDT            |
| 10  | Heptachlor epoxide       | 21  | p,p'-DDT            |
| 11  | Trans-heptachlor epoxide | 22  | Endosulfan sulfate  |

(Names of components in chromatogram are inferred according to files and experience)

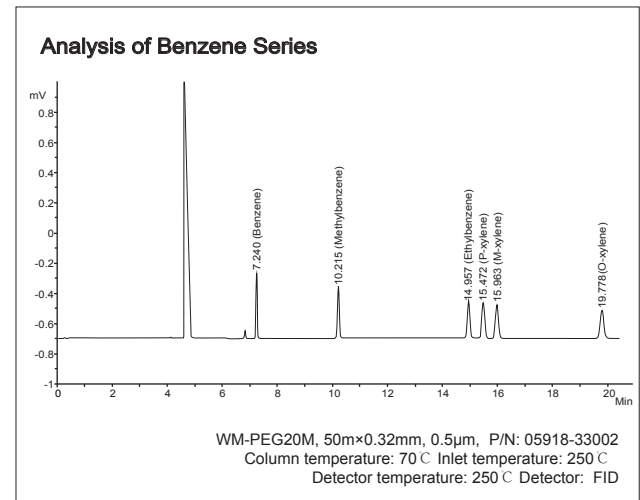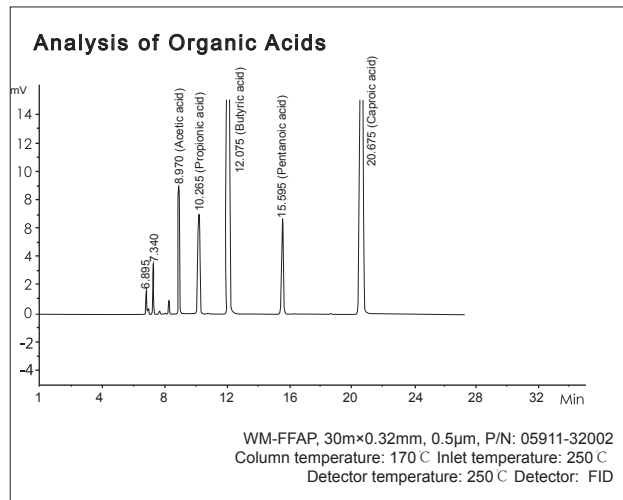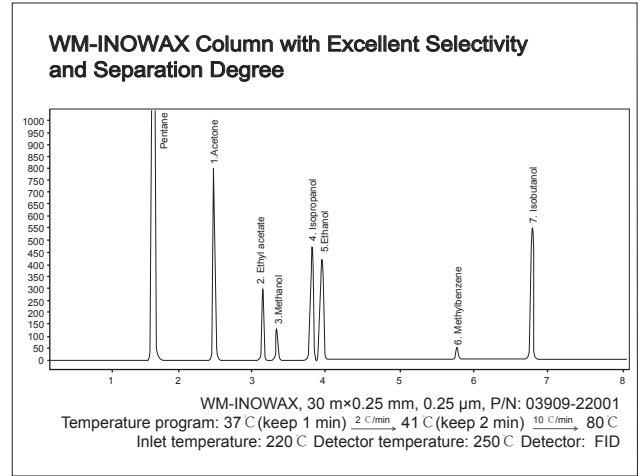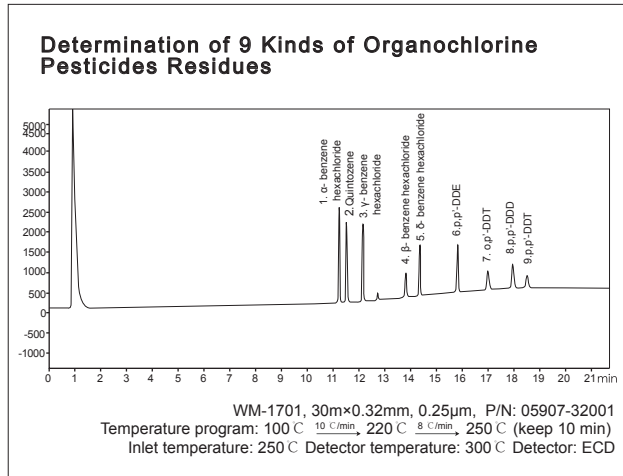

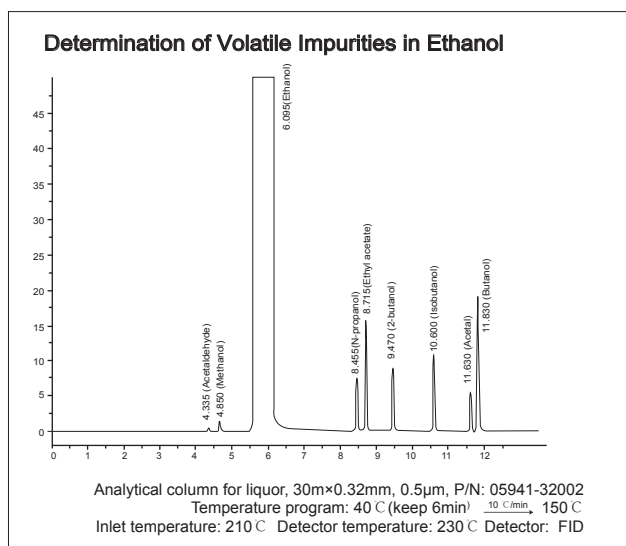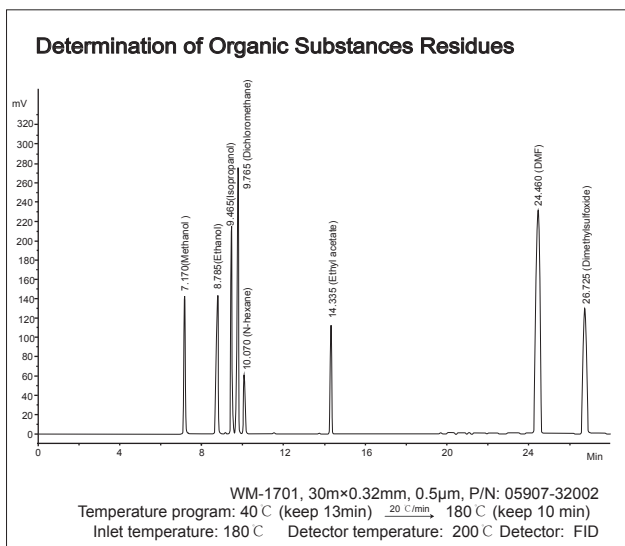

## Cross Reference

| Stationary Liquid | USP | Similar Stationary Liquid                                 |
|-------------------|-----|-----------------------------------------------------------|
| WM-1              | G2  | DB-1, HP-1, OV-1, BP-1, Rtx-1, OV-101, SPB-1, CP-Sil 5CB  |
| WM-1MS            | G2  | DB-1MS, HP-1MS, OV-1MS, OV-1MS                            |
| WM-5              | G27 | BP-5, ZB-5, CP-Sil 8CB, DB-5, HP-5, SPB-5, Rtx-5, OV-5    |
| WM-5MS            | G27 | ZB-5MS, DB-5MS, HP-5MS, OV-5MS                            |
| WM-35             | G42 | DB-35, HP-35, SPB-35, Rtx-35, PE-35, AT-35                |
| WM-1301           | G43 | DB-1301, HP-1301, PE-1301, Rtx-1301                       |
| WM-1701           | G46 | BP-10, CB-1701, CP-Sil 19CB, DB-1701, Rtx-1701            |
| WM-225            | G7  | 007-225, DB-225, BP-225, HP-225, CP-Sil 43CB, Rtx-225     |
| WM-624            | G43 | 007-624, AT-624, CP-624, DB-624, HP-624, Rtx-502.2, VOCOL |
| WM-INOWAX         | G16 | CP-Wax, DB-Wax, HP-Innowax, PE-Wax, Rtx-Wax               |
| WM-FFAP           | G35 | BP-21, HP-FFAP, PE-FFAP, CP-FFAP, DB-FFAP, Nukol          |
| WM-17             | G3  | DB-17, HP-17, HP-50, Rtx-50, AT-50, SPB-50, SP-2250       |

## Guideline of Selecting WM High Performance Series Capillary Column

| WM Type       | Stationary Phase Type                             | Polarity          | Temp. limit ( C ) | Application Range                                                                                |
|---------------|---------------------------------------------------|-------------------|-------------------|--------------------------------------------------------------------------------------------------|
| WM-1,WM-1MS   | 100% Dimethyl Polysiloxan                         | Nonpolarity       | -60 to 325/350    | Hydrocarbons, Aromatics, Pesticides, Phenols, Herbicides, Amines, Fatty Acid Methyl Esters, etc. |
| WM-5,WM-5MS   | 5% Phenyl, 95% Dimethyl Polysiloxane              | Weak polarity     | -60 to 325/350    | Hydrocarbons, Aromatics, Pesticides, Herbicides, Drugs, Biodiesel, etc.                          |
| WM-1301       | 6% Cyanopropyl-phenyl, 94% Dimethyl Polysiloxane  | Moderate polarity | -20 to 280/300    | Alcohols, Pesticides, VOCs, iodines, Pesticide Residues, etc.                                    |
| WM-35,WM-35MS | 35% Phenyl, 65% Dimethyl Polysiloxane             | Moderate polarity | 40 to 300/320     | Alcohols, Pesticides, Drugs                                                                      |
| WM-17,WM-17MS | 14% Cyanopropyl-phenyl, 86% Dimethyl Polysiloxane | Moderate polarity | 40 to 300/320     | Drugs, ethylene glycol, steroids, herbicides, pesticides                                         |
| WM-1701       | 6% Cyanopropyl, 94% Dimethyl Polysiloxane         | Moderate polarity | -20 to 280/300    | Aromatic chlorine, insecticide, herbicide                                                        |
| WM-624        | 6% Cyanopropyl, 94% Dimethyl polysiloxane         | Moderate polarity | -20 to 260        | Solvent residual, volatile compounds                                                             |
| WM-225        | 50% Cyanopropyl, 50% Dimethyl polysiloxane        | Moderate polarity | 40 to 220/240     | Neutral sterols, sugar alcohol acetate                                                           |

| WM Type   | Stationary Phase Type                           | Polarity        | Temp. limit (°C) | Application Range                                                                                      |
|-----------|-------------------------------------------------|-----------------|------------------|--------------------------------------------------------------------------------------------------------|
| WM-INOWAX | Polyethylene glycol                             | Strong polarity | 40 to 260/280    | Alcohols, Free Acids, Fatty Acid Methyl Esters, Polynuclears, Aromatics, Solvents, Essential Oils etc. |
| WM-FFAP   | Polyethylene glycol modified by p-Phthalic acid | Strong polarity | 50 to 260        | Alcohols, Free Acids, Fatty Acid Methyl Esters, Aldehydes, Acrylic Esters, Ketones, etc.               |

### WM High Performance Series Capillary Column WM-1, WM-1MS

- ▶ 100% Dimethyl polysiloxane stationary liquid
- ▶ General nonpolar stationary phase
- ▶ Thermal stability is up to 350°C
- ▶ Chemically bonded crosslinked columns can be flushed with solvent
- ▶ Polarity is similar to stationary phases of DB-1, SPB-1, HP-1, SE-30
- ▶ Comply with USP G2 specific stationary liquid
- ▶ As a kind of low-loss column, it can be used with MS detector

WM-1 capillary column which formed by the crosslink of 100% polydimethylsiloxane can separate samples by boiling point, so it is suitable in a wide range of temperature. Due to the covalent crosslinking method, WM-1 column is able to tolerate large injection volume while keeping a long lifetime.

Through a more rigorous manufacturing technique, WM-1MS capillary column has low loss rate. Before being a qualified product, each column needs to be strictly tested, which is assuring. With good inertness to active compounds, Ultra-low loss WM-1MS column can effectively improve the detection performance of MS, ECD and NPD.

### WM-1 Ordering Information

| Specification          | P/N         | Specification          | P/N         |
|------------------------|-------------|------------------------|-------------|
| WM-1 10m×0.18mm×0.18μm | 03901-80018 | WM-1 25m×0.2mm×0.33μm  | 03901-18021 |
| WM-1 20m×0.18mm×0.18μm | 03901-89018 | WM-1 25m×0.2mm×0.5μm   | 03901-18002 |
| WM-1 20m×0.18mm×0.36μm | 03901-89028 | WM-1 30m×0.25mm×0.1μm  | 03901-22007 |
| WM-1 20m×0.18mm×0.4μm  | 03901-89022 | WM-1 30m×0.25mm×0.25μm | 03901-22001 |
| WM-1 25m×0.2mm×0.11μm  | 03901-18029 | WM-1 30m×0.25mm×0.5μm  | 03901-22002 |

| Specification          | P/N         | Specification          | P/N         |
|------------------------|-------------|------------------------|-------------|
| WM-1 50m×0.32mm×0.17μm | 03901-33030 | WM-1 30m×0.2mm×0.5μm   | 05901-12002 |
| WM-1 15m×0.2mm×0.25μm  | 05901-11001 | WM-1 30m×0.25mm×0.25μm | 05901-22001 |
| WM-1 15m×0.2mm×0.5μm   | 05901-11002 | WM-1 30m×0.25mm×0.5μm  | 05901-22002 |
| WM-1 15m×0.25mm×0.25μm | 05901-21001 | WM-1 30m×0.32mm×0.25μm | 05901-32001 |
| WM-1 15m×0.25mm×0.5μm  | 05901-21002 | WM-1 30m×0.32mm×0.5μm  | 05901-32002 |
| WM-1 15m×0.32mm×0.25μm | 05901-31001 | WM-1 30m×0.32mm×1μm    | 05901-32003 |
| WM-1 15m×0.32mm×0.5μm  | 05901-31002 | WM-1 30m×0.53mm×0.5μm  | 05901-52002 |
| WM-1 15m×0.53mm×0.5μm  | 05901-51002 | WM-1 30m×0.53mm×1.0μm  | 05901-52003 |
| WM-1 30m×0.2mm×0.25μm  | 05901-12001 |                        |             |

### WM-1MS Ordering Information



| Specification            | P/N         | Specification            | P/N         |
|--------------------------|-------------|--------------------------|-------------|
| WM-1MS 20m×0.18mm×0.18μm | 03903-89018 | WM-1MS 30m×0.25mm×1.0μm  | 03903-22003 |
| WM-1MS 20m×0.18mm×0.36μm | 03903-89028 | WM-1MS 60m×0.25mm×0.25μm | 03903-24001 |
| WM-1MS 20m×0.18mm×0.4μm  | 03903-89022 | WM-1MS 15m×0.32mm×0.25μm | 03903-31001 |
| WM-1MS 15m×0.20mm×0.33μm | 03903-11021 | WM-1MS 25m×0.32mm×0.52μm | 03903-38024 |
| WM-1MS 25m×0.20mm×0.33μm | 03903-18021 | WM-1MS 30m×0.32mm×0.1μm  | 03903-32007 |
| WM-1MS 15m×0.25mm×0.25μm | 03903-21001 | WM-1MS 30m×0.32mm×0.25μm | 03903-32001 |
| WM-1MS 30m×0.25mm×0.1μm  | 03903-22007 | WM-1MS 30m×0.32mm×1.0μm  | 03903-32003 |
| WM-1MS 30m×0.25mm×0.25μm | 03903-22001 | WM-1MS 60m×0.32mm×0.25μm | 03903-34001 |
| WM-1MS 30m×0.25mm×0.5μm  | 03903-22002 | WM-1MS 60m×0.32mm×1.0μm  | 03903-34003 |

### WM-5,WM-54,WM-5MS

- ▶ 5% Diphenyl 95% dimethyl polysiloxane stationary liquid
- ▶ General low-polarity stationary phase
- ▶ Thermal stability is up to 350°C
- ▶ Chemically bonded crosslinked columns can be flushed with solvent
- ▶ Polarity is similar to stationary phases of DB-5, SPB-5, HP-5, Rtx-5
- ▶ Comply with USP G27 specific stationary liquid
- ▶ With low-loss, excellent inertness and high column efficiency,
- ▶ WM-5MS can be used with MS detector

Due to the addition of 5% diphenyl in polydimethylsiloxane, WM-5 column has higher polarity than WM-1 capillary column and has better selectivity to aromatic compounds. In most cases, it will be the type of column you first consider. Beside, WM-5 capillary column also has excellent reproducibility and high column efficiency.

Through a more rigorous manufacturing technique, WM-5MS capillary column has low loss rate. Before being a qualified product, each column needs to be strictly tested, which is assuring. With good inertness to active compounds, ultra-low loss WM-5MS column can effectively improve the detection performance of MS, ECD and NPD.

| Specification          | P/N         | Specification           | P/N         |
|------------------------|-------------|-------------------------|-------------|
| WM-5 30m×0.25mm×0.25μm | 05902-22001 | WM-5 50m×0.32m×0.5μm    | 05902-33002 |
| WM-5 50m×0.25mm×0.25μm | 05902-23001 | WM-54 15m×0.2mm×0.25μm  | 05915-11001 |
| WM-5 60m×0.25mm×0.5μm  | 05902-24002 | WM-54 15m×0.25mm×0.25μm | 05915-21001 |
| WM-5 30m×0.32mm×0.25μm | 05902-32001 | WM-54 30m×0.25mm×0.25μm | 05915-22001 |
| WM-5 30m×0.32m×0.5μm   | 05902-32002 | WM-54 30m×0.25mm×0.5μm  | 05915-22002 |

| Specification           | P/N         | Specification          | P/N         |
|-------------------------|-------------|------------------------|-------------|
| WM-54 50m×0.25mm×0.5μm  | 05915-23002 | WM-5 10m×0.18mm×0.36μm | 03902-80028 |
| WM-54 30m×0.32mm×0.25μm | 05915-32001 | WM-5 10m×0.18mm×0.4μm  | 03902-80022 |
| WM-54 30m×0.32mm×0.5μm  | 05915-32002 | WM-5 20m×0.18mm×0.18μm | 03902-89018 |
| WM-54 30m×0.32mm×1.0μm  | 05915-32003 | WM-5 20m×0.18mm×0.4μm  | 03902-89022 |
| WM-54 30m×0.53mm×0.5μm  | 05915-52002 | WM-5 25m×0.20mm×0.11μm | 03902-18029 |
| WM-54 30m×0.53mm×3.0μm  | 05915-52006 | WM-5 25m×0.20mm×0.33μm | 03902-18021 |
| WM-5 10m×0.18mm×0.18μm  | 03902-80018 |                        |             |

| Specification           | P/N         |
|-------------------------|-------------|
| WM-54 50m×0.25mm×0.5μm  | 05915-23002 |
| WM-54 30m×0.32mm×0.25μm | 05915-32001 |
| WM-54 30m×0.32mm×0.5μm  | 05915-32002 |
| WM-54 30m×0.32mm×1.0μm  | 05915-32003 |
| WM-54 30m×0.53mm×0.5μm  | 05915-52002 |
| WM-54 30m×0.53mm×3.0μm  | 05915-52006 |
| WM-5 10m×0.18mm×0.18μm  | 03902-80018 |

| Specification          | P/N         |
|------------------------|-------------|
| WM-5 10m×0.18mm×0.36μm | 03902-80028 |
| WM-5 10m×0.18mm×0.4μm  | 03902-80022 |
| WM-5 20m×0.18mm×0.18μm | 03902-89018 |
| WM-5 20m×0.18mm×0.4μm  | 03902-89022 |
| WM-5 25m×0.20mm×0.11μm | 03902-18029 |
| WM-5 25m×0.20mm×0.33μm | 03902-18021 |

### WM-5MS Ordering Information:

| Specification            | P/N         |
|--------------------------|-------------|
| WM-5MS 10m×0.1mm×0.1μm   | 03904-00007 |
| WM-5MS 10m×0.18mm×0.18μm | 03904-80018 |
| WM-5MS 20m×0.18mm×0.18μm | 03904-89018 |
| WM-5MS 20m×0.18mm×0.36μm | 03904-89028 |
| WM-5MS 25m×0.20mm×0.33μm | 03904-18021 |
| WM-5MS 15m×0.25mm×0.1μm  | 03904-21007 |
| WM-5MS 15m×0.25mm×0.25μm | 03904-21001 |
| WM-5MS 15m×0.25mm×0.5μm  | 03904-21002 |
| WM-5MS 15m×0.25mm×1.0μm  | 03904-21003 |
| WM-5MS 30m×0.25mm×0.1μm  | 03904-22007 |
| WM-5MS 30m×0.25mm×0.25μm | 03904-22001 |
| WM-5MS 30m×0.25mm×0.5μm  | 03904-22002 |
| WM-5MS 30m×0.25mm×1.0μm  | 03904-22003 |
| WM-5MS 60m×0.25mm×0.1μm  | 03904-24007 |
| WM-5MS 60m×0.25mm×0.25μm | 03904-24001 |

| Specification            | P/N         |
|--------------------------|-------------|
| WM-5MS 60m×0.25mm×0.5μm  | 03904-24002 |
| WM-5MS 60m×0.25mm×1.0μm  | 03904-24003 |
| WM-5MS 15m×0.32mm×0.1μm  | 03904-31007 |
| WM-5MS 15m×0.32mm×0.25μm | 03904-31001 |
| WM-5MS 15m×0.32mm×0.5μm  | 03904-31002 |
| WM-5MS 15m×0.32mm×1.0μm  | 03904-31003 |
| WM-5MS 25m×0.32mm×0.52μm | 03904-38024 |
| WM-5MS 30m×0.32mm×0.1μm  | 03904-32007 |
| WM-5MS,30m×0.32mm×0.25μm | 03904-32001 |
| WM-5MS 30m×0.32mm×0.5μm  | 03904-32002 |
| WM-5MS 30m×0.32mm×1.0μm  | 03904-32003 |
| WM-5MS 60m×0.32mm×0.1μm  | 03904-34007 |
| WM-5MS 60m×0.32mm×0.25μm | 03904-34001 |
| WM-5MS 60m×0.32mm×0.5μm  | 03904-34002 |
| WM-5MS 60m×0.32mm×1.0μm  | 03904-34003 |

### WM-1301,WM-624

- ▶ 6% Cyanopropyl phenyl,94% dimethyl polysiloxane
- ▶ Comply with USP G43 specific stationary liquid
- ▶ It is specially used for the analysis of volatile organic compounds and residual solvents in drugs
- ▶ Bond and crosslink with medium polarity
- ▶ Has Excellent inertness for most compounds
- ▶ Temperature range: -20 to 260 C
- ▶ Polarity is similar to stationary phases of DB-624, SPB-1301, HP-624, Elite-1301, Rtx-624.
- ▶ WM-624 is specially designed for EPA method

### WM-1301 Ordering Information:

| Specification             | P/N         |
|---------------------------|-------------|
| WM-1301 15m×0.25mm×0.25μm | 03905-21001 |
| WM-1301 30m×0.25mm×0.25μm | 03905-22001 |
| WM-1301 30m×0.25mm×0.5μm  | 03905-22002 |

| Specification             | P/N         |
|---------------------------|-------------|
| WM-1301 30m×0.25mm×1.0μm  | 03905-22003 |
| WM-1301 60m×0.25mm×0.25μm | 03905-24001 |
| WM-1301 60m×0.25mm×1.0μm  | 03905-24003 |

| Specification             | P/N         | Specification             | P/N         |
|---------------------------|-------------|---------------------------|-------------|
| WM-1301 60m×0.25mm×1.4μm  | 03905-24009 | WM-1301 15m×0.32mm×0.5μm  | 05905-31002 |
| WM-1301 15m×0.32mm×0.25μm | 03905-31001 | WM-1301 15m×0.53mm×0.5μm  | 05905-51002 |
| WM-1301 15m×0.32mm×0.5μm  | 03905-31002 | WM-1301 30m×0.2mm×0.25μm  | 05905-12001 |
| WM-1301 30m×0.32mm×0.25μm | 03905-32001 | WM-1301 30m×0.2mm×0.5μm   | 05905-12002 |
| WM-1301 30m×0.32mm×0.5μm  | 03905-32002 | WM-1301 30m×0.25mm×0.25μm | 05905-22001 |
| WM-1301 30m×0.32mm×1.0μm  | 03905-32003 | WM-1301 30m×0.25mm×0.5μm  | 05905-22002 |
| WM-1301 15m×0.2mm×0.25μm  | 05905-11001 | WM-1301 30m×0.25mm×1.4μm  | 05905-22009 |
| WM-1301 15m×0.2mm×0.5μm   | 05905-11002 | WM-1301 30m×0.32mm×0.25μm | 05905-32001 |
| WM-1301 15m×0.25mm×0.25μm | 05905-21001 | WM-1301 30m×0.32mm×0.5μm  | 05905-32002 |
| WM-1301 15m×0.25mm×0.5μm  | 05905-21002 | WM-1301 50m×0.2mm×0.5μm   | 05905-13002 |
| WM-1301 30m×0.25mm×1μm    | 05905-22003 | WM-1301 50m×0.25mm×0.25μm | 05905-23001 |
| WM-1301 15m×0.32mm×0.25μm | 05905-31001 |                           |             |

**WM-624 Ordering Information:**

| Specification            | P/N          | Product             |
|--------------------------|--------------|---------------------|
| WM-624 30m×0.25mm×1.4μm  | 03908-22009  | GC capillary column |
| WM-624 60m×0.25mm×1.4μm  | 03908-24009  | GC capillary column |
| WM-624 30m×0.32mm×0.25μm | 03908-32001  | GC capillary column |
| WM-624 30m×0.32mm×1.8μm  | 03908-32004  | GC capillary column |
| WM-624 60m×0.32mm×1.8μm  | 03908-34004  | GC capillary column |
| WM-624 30m×0.53mm×3.0μm  | 03908-52006  | GC capillary column |
| WM-624 60m×0.53mm×3.0μm  | 03908-54006  | GC capillary column |
| WM-624 60m×0.53mm×3.0μm  | 05908-54006  | GC capillary column |
| WM-624 20m×0.18mm×1.0μm  | 03908-89003  | GC capillary column |
| WM-624 75m×0.53mm×3.0μm  | 03908-512006 | GC capillary column |

**WM-35,WM-35MS**

- ▶ 35% Diphenyl 65% dimethyl polysiloxane stationary liquid
- ▶ General low-polarity stationary phase
- ▶ Thermal stability is up to 320 C
- ▶ Chemically bonded crosslinked columns can be flushed with solvent
- ▶ Polarity is similar to stationary phases of DB-35, SPB-35, HP-35, Rtx-35, PE-35
- ▶ Comply with USP G42 specific stationary liquid
- ▶ As a kind of low-loss column, it can be used with MS detector

Due to the addition of 35% diphenyl in polydimethylsiloxane, WM-35 column is suitable for the analysis of compounds with medium polarity. Besides, WM-35 capillary column has excellent reproducibility and high column efficiency.

Through a more rigorous manufacturing technique, WM-35MS capillary has low loss rate. Before being a qualified product, each column needs to be strictly tested, which is assuring. With good inertness to active compounds, Ultra-low loss WM-35MS column can effectively improve the detection performance of MS, ECD and NPD.

**WM-35 Ordering Information:**

| Specification           | P/N         |
|-------------------------|-------------|
| WM-35 20m×0.18mm×0.18μm | 03921-89018 |
| WM-35 15m×0.20mm×0.33μm | 03921-11021 |
| WM-35 25m×0.20mm×0.33μm | 03921-18021 |
| WM-35 30m×0.25mm×0.15μm | 03921-22008 |
| WM-35 30m×0.25mm×0.5μm  | 03921-22002 |
| WM-35 60m×0.25mm×0.25μm | 03921-24001 |
| WM-35 60m×0.32mm×0.25μm | 03921-24002 |
| WM-35 15m×0.32mm×0.25μm | 03921-31001 |

| Specification           | P/N         |
|-------------------------|-------------|
| WM-35 30m×0.32mm×0.25μm | 03921-32001 |
| WM-35 30m×0.32mm×1.0μm  | 03921-32003 |
| WM-35 60m×0.32mm×0.25μm | 03921-34001 |
| WM-35 60m×0.32mm×0.5μm  | 03921-34002 |
| WM-35 30m×0.53mm×0.5μm  | 03921-52002 |
| WM-35 30m×0.53mm×1.5μm  | 03921-52025 |
| WM-35 60m×0.53mm×0.5μm  | 03921-54002 |

**WM-35MS Ordering Information:**

| Specification             | P/N         |
|---------------------------|-------------|
| WM-35MS 20m×0.18mm×0.18μm | 03906-89018 |
| WM-35MS 15m×0.20mm×0.33μm | 03906-11021 |
| WM-35MS 25m×0.20mm×0.33μm | 03906-18021 |
| WM-35MS 15m×0.25mm×0.25μm | 03906-21001 |
| WM-35MS 30m×0.25mm×0.15μm | 03906-22008 |
| WM-35MS 30m×0.25mm×0.25μm | 03906-22001 |

| Specification             | P/N         |
|---------------------------|-------------|
| WM-35MS 60m×0.25mm×0.25μm | 03906-24001 |
| WM-35MS 15m×0.32mm×0.25μm | 03906-31001 |
| WM-35MS 30m×0.32mm×0.25μm | 03906-32001 |
| WM-35MS 30m×0.53mm×0.5μm  | 03906-52002 |
| WM-35MS 30m×0.53mm×1.0μm  | 03906-52003 |

**WM-17,WM-17MS**

- ▶ 50% diphenyl 50% dimethyl polysiloxane
- ▶ General low-polarity stationary phase
- ▶ Thermal stability is up to 320 °C
- ▶ Chemically bonded crosslinked columns can be flushed with solvent
- ▶ Polarity is similar to stationary phases of DB-17, HP-17, SPB-50
- ▶ Comply with USP G3 specific stationary liquid
- ▶ Low-loss WM-17MS can be used with MS detector

Due to the addition of 50% diphenyl in polydimethylsiloxane, WM-17 column is suitable for the analysis of compounds with medium polarity. Besides, WM-17 capillary column has excellent reproducibility and high column efficiency.

Through a more rigorous manufacturing technique, WM-17 capillary column has low loss rate. Before being a qualified product, each column needs to be strictly tested, which is assuring. With good inertness to active compounds, ultra-low loss WM-17 column can effectively improve the detection performance of MS, ECD and NPD.

| Specification           | P/N         |
|-------------------------|-------------|
| WM-17 20m×0.18mm×0.18μm | 03916-89018 |
| WM-17 20m×0.18mm×0.3μm  | 03916-89013 |
| WM-17 15m×0.25mm×0.15μm | 03916-21008 |
| WM-17 15m×0.25mm×0.25μm | 03916-21001 |
| WM-17 15m×0.25mm×0.5μm  | 03916-21002 |
| WM-17 30m×0.25mm×0.15μm | 03916-22008 |
| WM-17 30m×0.25mm×0.25μm | 03916-22001 |

| Specification           | P/N         |
|-------------------------|-------------|
| WM-17 15m×0.32mm×0.15μm | 03916-31008 |
| WM-17 15m×0.32mm×0.25μm | 03916-31001 |
| WM-17 15m×0.32mm×0.5μm  | 03916-31002 |
| WM-17 30m×0.32mm×0.15μm | 03916-32008 |
| WM-17 30m×0.32mm×0.25μm | 03916-32001 |
| WM-17 60m×0.32mm×0.5μm  | 05916-34002 |
| WM-17 30m×0.53mm×1.0μm  | 05916-52003 |

| Specification           | P/N         |
|-------------------------|-------------|
| WM-17 30m×0.25mm×0.5μm  | 03916-22002 |
| WM-17 60m×0.25mm×0.25μm | 03916-24001 |

| Specification           | P/N         |
|-------------------------|-------------|
| WM-17 30m×0.25mm×0.25μm | 05916-22001 |
| WM-17 30m×0.32mm×0.25μm | 05916-32001 |

### WM-17MS Ordering Information:

| Specification             | P/N         |
|---------------------------|-------------|
| WM-17MS 20m×0.18mm×0.18μm | 03947-89018 |
| WM-17MS 15m×0.25mm×0.15μm | 03947-21008 |
| WM-17MS 15m×0.25mm×0.25μm | 03947-21001 |
| WM-17MS 30m×0.25mm×0.15μm | 03947-22008 |
| WM-17MS 30m×0.25mm×0.25μm | 03947-22001 |
| WM-17MS 60m×0.25mm×0.25μm | 03947-24001 |

| Specification             | P/N         |
|---------------------------|-------------|
| WM-17MS 15m×0.32mm×0.25μm | 03947-31001 |
| WM-17MS 30m×0.32mm×0.25μm | 03947-32001 |
| WM-17MS 60m×0.32mm×0.25μm | 03947-34001 |
| WM-17MS 30m×0.53mm×0.5μm  | 03947-52002 |
| WM-17MS 15m×0.53mm×1.0μm  | 03947-51003 |

### WM-1701

- ▶ 14% Cyanopropylphenyl 86% dimethyl polysiloxane
- ▶ General medium-polarity stationary phase
- ▶ Thermal stability is up to 300 °C
- ▶ Chemically bonded crosslinked columns can be flushed with solvent
- ▶ Polarity is similar to stationary phases of DB-1701, SPB-1701, HP-1701
- ▶ Comply with USP G46 specific stationary liquid

### WM-1701 Ordering Information:

| Specification             | P/N         |
|---------------------------|-------------|
| WM-1701 30m×0.25mm×0.25μm | 05907-22001 |
| WM-1701 30m×0.25mm×0.5μm  | 05907-22002 |
| WM-1701 15m×0.32mm×0.25μm | 05907-31001 |
| WM-1701 30m×0.32mm×0.25μm | 05907-32001 |
| WM-1701 30m×0.32mm×0.5μm  | 05907-32002 |
| WM-1701 30m×0.32mm×2.65μm | 05907-32034 |
| WM-1701 50m×0.32mm×0.5μm  | 05907-33002 |
| WM-1701 15m×0.53mm×0.5μm  | 05907-51002 |
| WM-1701 20m×0.18mm×0.18μm | 03907-89018 |
| WM-1701 25m×0.20mm×0.2μm  | 03907-18011 |
| WM-1701 15m×0.25mm×0.25μm | 03907-21001 |
| WM-1701 30m×0.25mm×0.25μm | 03907-22001 |

| Specification             | P/N         |
|---------------------------|-------------|
| WM-1701 30m×0.25mm×0.5μm  | 03907-22002 |
| WM-1701 30m×0.25mm×1.0μm  | 03907-22003 |
| WM-1701 60m×0.25mm×0.25μm | 03907-24001 |
| WM-1701 60m×0.25mm×0.5μm  | 03907-24002 |
| WM-1701 15m×0.32mm×0.25μm | 03907-31001 |
| WM-1701 15m×0.32mm×0.5μm  | 03907-31002 |
| WM-1701 30m×0.32mm×0.25μm | 03907-32001 |
| WM-1701 30m×0.32mm×0.5μm  | 03907-32002 |
| WM-1701 30m×0.32mm×1.0μm  | 03907-32003 |
| WM-1701 60m×0.32mm×0.25μm | 03907-34001 |
| WM-1701 60m×0.32mm×0.5μm  | 03907-34002 |
| WM-1701 60m×0.32mm×1.0μm  | 03907-34003 |

### WM-225

- ▶ 50% Cyanopropylphenyl, 50% dimethyl polysiloxane
- ▶ Bonded crosslinked column
- ▶ Thermal stability is up to 240 °C
- ▶ Equivalent to USP stationary G7
- ▶ Stationary phase with medium polarity, suitable for separation of Cis or trans fatty acid methyl ester
- ▶ Polarity is similar to DB-225, HP-225, Rtx-225

**WM-225 Ordering Information:**

| Specification           | P/N         | Product             |
|-------------------------|-------------|---------------------|
| WM-225 30m×0.53mm×1.0μm | 05919-52003 | GC capillary column |

**WM-INOWAX**

- ▶ Bonded crosslinked polyethylene glycol (PEG)
- ▶ General stationary phase with polarity
- ▶ With antioxidant properties
- ▶ Thermal stability is up to 280 °C
- ▶ Chemically bonded crosslinked columns can be flushed with solvent
- ▶ Polarity is similar to stationary phases of HP-INNOWax, CP-WAX 52CB
- ▶ Comply with USP G16 specific stationary liquid

**WM-INOWAX Ordering Information**

| Specification               | P/N         | Specification               | P/N         |
|-----------------------------|-------------|-----------------------------|-------------|
| WM-INOWAX 10m×0.18mm×0.18μm | 03909-80018 | WM-INOWAX 60m×0.25mm×0.5μm  | 03909-24002 |
| WM-INOWAX 20m×0.18mm×0.18μm | 03909-89018 | WM-INOWAX 15m×0.32mm×0.25μm | 03909-31001 |
| WM-INOWAX 25m×0.20mm×0.2μm  | 03909-18011 | WM-INOWAX 15m×0.32mm×0.5μm  | 03909-31002 |
| WM-INOWAX 25m×0.20mm×0.4μm  | 03909-18022 | WM-INOWAX 30m×0.32mm×0.15μm | 03909-32008 |
| WM-INOWAX 50m×0.20mm×0.2μm  | 03909-13011 | WM-INOWAX 30m×0.32mm×0.25μm | 03909-32001 |
| WM-INOWAX 50m×0.20mm×0.4μm  | 03909-13022 | WM-INOWAX 30m×0.32mm×0.5μm  | 03909-32002 |
| WM-INOWAX 15m×0.25mm×0.25μm | 03909-21001 | WM-INOWAX 30m×0.32mm×1.0μm  | 03909-32003 |
| WM-INOWAX 15m×0.25mm×0.5μm  | 03909-21002 | WM-INOWAX 60m×0.32mm×0.15μm | 03909-34008 |
| WM-INOWAX 30m×0.25mm×0.15μm | 03909-22008 | WM-INOWAX 30m×0.53mm×1.0μm  | 03909-52003 |
| WM-INOWAX 30m×0.25mm×0.25μm | 03909-22001 | WM-INOWAX 60m×0.53mm×0.5μm  | 03909-54002 |
| WM-INOWAX 30m×0.25mm×0.5μm  | 03909-22002 | WM-INOWAX 50m×0.53mm×2.0μm  | 05909-53005 |
| WM-INOWAX 60m×0.25mm×0.15μm | 03909-24008 | WM-INOWAX 30m×0.25mm×0.25μm | 05909-22001 |
| WM-INOWAX 60m×0.25mm×0.25μm | 03909-24001 |                             |             |

**WM-FFAP**

- ▶ Nitroterephthalic acid modified polyethylene glycol
- ▶ Stationary phase has strong polarity
- ▶ Has special advantages in the analysis of volatile fatty acids and phenol and other substances
- ▶ Thermal stability is up to 260 °C
- ▶ Polarity is similar to stationary phases of DB-FFAP, HP-FFAP, Stabilwax-DA
- ▶ Comply with USP G35 specific stationary liquid

**WM-FFAP Ordering Information**

| Specification             | P/N         | Specification             | P/N         |
|---------------------------|-------------|---------------------------|-------------|
| WM-FFAP 30m×0.20mm×0.25μm | 05911-12001 | WM-FFAP 50m×0.20mm×0.3μm  | 03911-13013 |
| WM-FFAP 30m×0.25mm×0.25μm | 05911-22001 | WM-FFAP 15m×0.25mm×0.25μm | 03911-21001 |
| WM-FFAP 60m×0.25mm×0.25μm | 05911-24001 | WM-FFAP 30m×0.25mm×0.25μm | 03911-22001 |
| WM-FFAP 30m×0.32mm×0.25μm | 05911-32001 | WM-FFAP 30m×0.20mm×0.25μm | 03911-12001 |
| WM-FFAP 30m×0.32mm×0.5μm  | 05911-32002 | WM-FFAP 50m×0.25mm×0.25μm | 03911-23001 |
| WM-FFAP 30m×0.32mm×1.0μm  | 05911-32003 | WM-FFAP 15m×0.32mm×0.25μm | 03911-31001 |

| Specification             | P/N         |
|---------------------------|-------------|
| WM-FFAP 30m×0.53mm×0.5μm  | 05911-52002 |
| WM-FFAP 30m×0.53mm×1.0μm  | 05911-52003 |
| WM-FFAP 20m×0.18mm×0.18μm | 03911-89018 |
| WM-FFAP 25m×0.20mm×0.3μm  | 03911-18013 |

| Specification             | P/N         |
|---------------------------|-------------|
| WM-FFAP 25m×0.32mm×0.5μm  | 03911-38002 |
| WM-FFAP 30m×0.32mm×0.25μm | 03911-32001 |
| WM-FFAP 30m×0.32mm×0.5μm  | 03911-32002 |
| WM-FFAP 30m×0.32mm×1.0μm  | 03911-32003 |

| Specification             | P/N         |
|---------------------------|-------------|
| WM-FFAP 50m×0.32mm×0.5μm  | 03911-33002 |
| WM-FFAP 60m×0.32mm×0.25μm | 03911-34001 |

| Specification            | P/N         |
|--------------------------|-------------|
| WM-FFAP 10m×0.53mm×1.0μm | 03911-50003 |

## 1.2 WEL Series Economical GC Column


Each of the WEL series of capillary columns has been strictly tested with attached evaluation chromatogram. For high column efficiency and sensitivity, our products are popular among new and regular customers. We can provide sample analysis for customers to ensure the superior performance of columns and various dedicated columns for some test items with higher column efficiency and separation effect, which can help in the qualitative and quantitative analysis.

### Sample analysis flow




### Chromatogram of Typical Applications

#### 1. Detection of Volatile Impurities in Ethanol


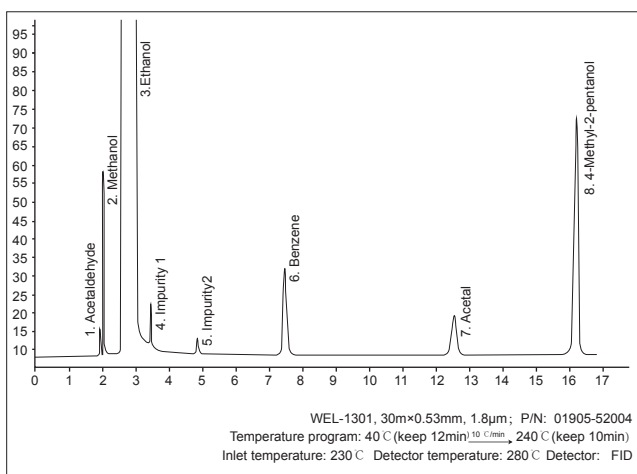


#### 2. Detection of Ethylene Glycol, Diethylene Glycol and Triethylene Glycol in Polyethylene Glycol 400

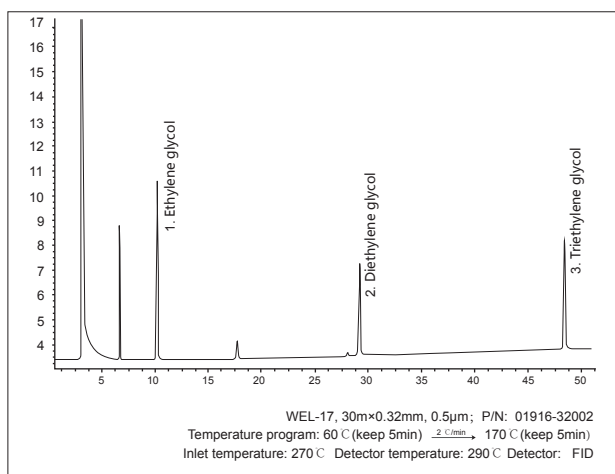


#### 3) Determination of Effective Composition of Borneol


#### 4) Analysis of Chloroalkanes

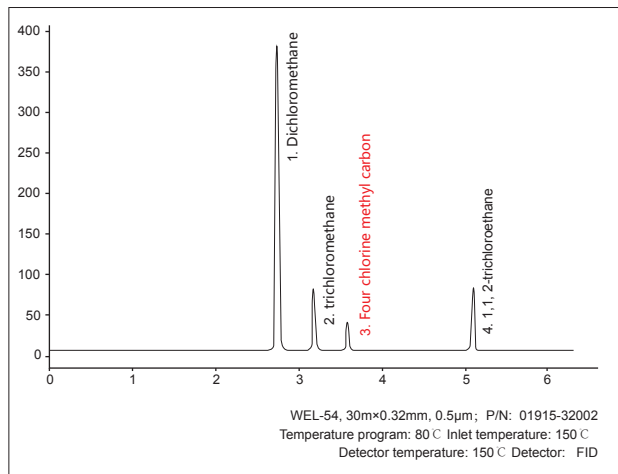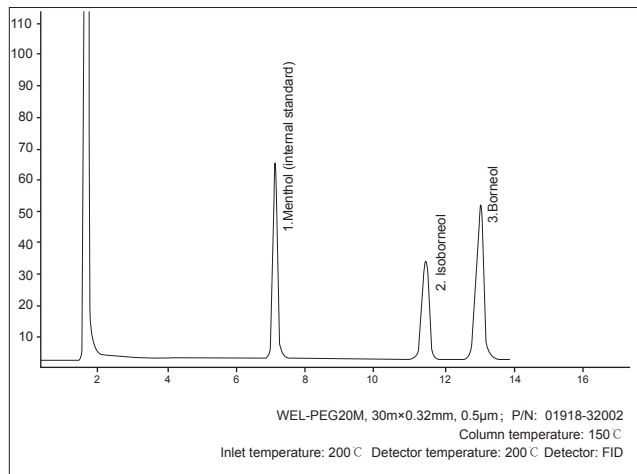

## 5) Determination of Ethyl Bromoacetate

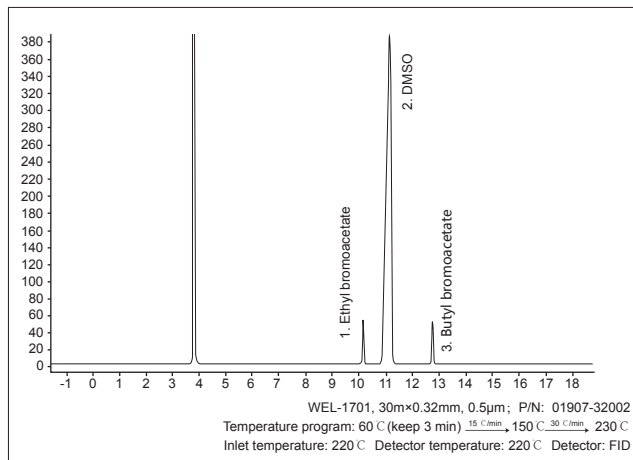

## 6) Determination of Organic Solvent Residue

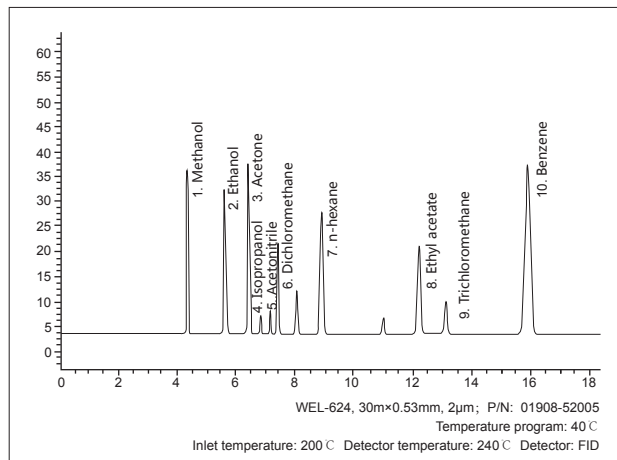

## Ordering Information

| Specification           | P/N         |
|-------------------------|-------------|
| WEL-1 30m×0.25mm×0.25µm | 01901-22001 |
| WEL-1 30m×0.25mm×0.5µm  | 01901-22002 |
| WEL-1 30m×0.25mm×1.0µm  | 01901-22003 |
| WEL-1 50m×0.25mm×0.25µm | 01901-23001 |
| WEL-1 50m×0.25mm×0.5µm  | 01901-23002 |
| WEL-1 50m×0.25mm×1.0µm  | 01901-23003 |
| WEL-1 60m×0.25mm×0.25µm | 01901-24001 |
| WEL-1 60m×0.25mm×0.5µm  | 01901-24002 |
| WEL-1 60m×0.25mm×1.0µm  | 01901-24003 |
| WEL-5 30m×0.32mm×0.25µm | 01902-32001 |
| WEL-5 30m×0.32mm×0.5µm  | 01902-32002 |
| WEL-5 30m×0.32mm×1.0µm  | 01902-32003 |
| WEL-5 30m×0.32mm×3.0µm  | 01902-32006 |

| Specification              | P/N         |
|----------------------------|-------------|
| WEL-1701 50m×0.25mm×0.25µm | 01907-23001 |
| WEL-1701 50m×0.25mm×0.5µm  | 01907-23002 |
| WEL-1701 50m×0.25mm×1.0µm  | 01907-23003 |
| WEL-1701 60m×0.25mm×0.25µm | 01907-24001 |
| WEL-1701 60m×0.25mm×0.5µm  | 01907-24002 |
| WEL-624 30m×0.25mm×0.25µm  | 01908-22001 |
| WEL-624 30m×0.25mm×0.5µm   | 01908-22002 |
| WEL-624 30m×0.25mm×1.0µm   | 01908-22003 |
| WEL-624 30m×0.25mm×1.4µm   | 01908-22004 |
| WEL-624 50m×0.25mm×0.25µm  | 01908-23001 |
| WEL-624 50m×0.25mm×0.5µm   | 01908-23002 |
| WEL-624 50m×0.25mm×1.0µm   | 01908-23003 |
| WEL-624 60m×0.25mm×0.25µm  | 01908-24001 |



| Specification              | P/N         |
|----------------------------|-------------|
| WEL-5 15m×0.53mm×1.0μm     | 01902-51003 |
| WEL-5 30m×0.53mm×1.0μm     | 01902-52003 |
| WEL-5 50m×0.53mm×1.0μm     | 01902-53003 |
| WEL-1301 60m×0.25mm×1.8μm  | 01905-24004 |
| WEL-1301 30m×0.32mm×1.8μm  | 01905-32004 |
| WEL-1301 30m×0.53mm×1.8μm  | 01905-52004 |
| WEL-1301 50m×0.53mm×2.0μm  | 01905-53005 |
| WEL-1301 30m×0.53mm×2.0μm  | 01905-52005 |
| WEL-1701 30m×0.25mm×0.25μm | 01907-22001 |
| WEL-1701 30m×0.25mm×0.5μm  | 01907-22002 |
| WEL-1701 30m×0.25mm×1.0μm  | 01907-22003 |

| Specification              | P/N         |
|----------------------------|-------------|
| WEL-624 60m×0.25mm×0.5μm   | 01908-24002 |
| WEL-624 60m×0.25mm×1.0μm   | 01908-24003 |
| WEL-624 25m×0.25mm×0.2μm   | 01908-28011 |
| WEL-624 30m×0.32mm×0.25μm  | 01908-32001 |
| WEL-624 30m×0.32mm×0.5μm   | 01908-32002 |
| WEL-FFAP 30m×0.25mm×0.25μm | 01911-22001 |
| WEL-FFAP 30m×0.25mm×0.5μm  | 01911-22002 |
| WEL-FFAP 30m×0.25mm×1.0μm  | 01911-22003 |
| WEL-FFAP 50m×0.25mm×0.5μm  | 01911-23002 |
| WEL-FFAP 50mm×0.25mm×1.0μm | 01911-23003 |
| WEL-FFAP 60m×0.25mm×0.25μm | 01911-24001 |

| Specification              | P/N         |
|----------------------------|-------------|
| WEL-FFAP 60m×0.25mm×0.5μm  | 01911-24002 |
| WEL-FFAP 60m×0.25mm×1.0μm  | 01911-24003 |
| WEL-FFAP 30m×0.32mm×0.25μm | 01911-32001 |
| WEL-FFAP 30m×0.32mm×0.5μm  | 01911-32002 |
| WEL-FFAP 30m×0.32mm×1.0μm  | 01911-32003 |
| WEL-FFAP 50m×0.32mm×0.25μm | 01911-33001 |
| WEL-FFAP 50m×0.32mm×0.5μm  | 01911-33002 |
| WEL-FFAP 50m×0.32mm×1.0μm  | 01911-33003 |
| WEL-30 30m×0.25mm×0.25μm   | 01912-22001 |
| WEL-30 30m×0.25mm×0.5μm    | 01912-22002 |
| WEL-30 30m×0.25mm×1.0μm    | 01912-22003 |
| WEL-30 50m×0.25mm×0.25μm   | 01912-23001 |
| WEL-30 50m×0.25mm×0.5μm    | 01912-23002 |
| WEL-30 50m×0.25mm×1.0μm    | 01912-23003 |
| WEL-30 60m×0.25mm×0.25μm   | 01912-24001 |
| WEL-30 60m×0.25mm×0.5μm    | 01912-24002 |
| WEL-30 60m×0.25mm×1.0μm    | 01912-24003 |
| WEL-30 30m×0.32mm×0.25μm   | 01912-32001 |
| WEL-30 30m×0.32mm×0.5μm    | 01912-32002 |

| Specification             | P/N         |
|---------------------------|-------------|
| WEL-30 30m×0.32mm×1.0μm   | 01912-32003 |
| WEL-30 50m×0.32mm×0.25μm  | 01912-33001 |
| WEL-101 30m×0.25mm×0.25μm | 01913-22001 |
| WEL-101 30m×0.25mm×0.5μm  | 01913-22002 |
| WEL-101 30m×0.25mm×1.0μm  | 01913-22003 |
| WEL-101 50m×0.25mm×0.25μm | 01913-23001 |
| WEL-101 50m×0.25mm×0.5μm  | 01913-23002 |
| WEL-101 50m×0.25mm×1.0μm  | 01913-23003 |
| WEL-101 60m×0.25mm×0.25μm | 01913-24001 |
| WEL-101 60m×0.25mm×0.5μm  | 01913-24002 |
| WEL-101 60m×0.25mm×1.0μm  | 01913-24003 |
| WEL-101 30m×0.32mm×0.25μm | 01913-32001 |
| WEL-101 30m×0.32mm×0.5μm  | 01913-32002 |
| WEL-101 30m×0.32mm×1.0μm  | 01913-32003 |
| WEL-101 50m×0.32mm×0.25μm | 01913-33001 |
| WEL-101 50m×0.32mm×0.5μm  | 01913-33002 |
| WEL-52 30m×0.32mm×0.25μm  | 01914-32001 |
| WEL-54 50m×0.25mm×0.25μm  | 01915-23001 |
| WEL-54 50m×0.25mm×0.5μm   | 01915-23002 |

| Specification            | P/N         |
|--------------------------|-------------|
| WEL-17 50m×0.25mm×1.0μm  | 01916-23003 |
| WEL-17 60m×0.25mm×0.25μm | 01916-24001 |
| WEL-17 60m×0.25mm×0.5μm  | 01916-24002 |
| WEL-54 60m×0.25mm×1.0μm  | 01915-24003 |

| Specification             | P/N         |
|---------------------------|-------------|
| WEL-XE60 50m×0.32mm×0.5μm | 01917-33002 |
| WEL-XE60 50m×0.32mm×1.0μm | 01917-33003 |
| WEL-225 30m×0.25mm×0.25μm | 01919-22001 |
| WEL-17 30m×0.32mm×1.0μm   | 01916-32003 |

| Specification            | P/N         |
|--------------------------|-------------|
| WEL-54 30m×0.32mm×0.25µm | 01915-32001 |
| WEL-54 30m×0.32mm×0.5µm  | 01915-32002 |
| WEL-54 30m×0.32mm×1.0µm  | 01915-32003 |
| WEL-54 50m×0.32mm×0.25µm | 01915-33001 |
| WEL-54 50m×0.32mm×0.5µm  | 01915-33002 |
| WEL-54 50m×0.32mm×1.0µm  | 01915-33003 |
| WEL-17 30m×0.25mm×0.25µm | 01916-22001 |
| WEL-17 30m×0.25mm×0.5µm  | 01916-22002 |
| WEL-17 30m×0.25mm×1.0µm  | 01916-22003 |
| WEL-17 50m×0.25mm×0.25µm | 01916-23001 |
| WEL-17 50m×0.25mm×0.5µm  | 01916-23002 |
| WEL-17 50m×0.25mm×1.0µm  | 01916-23003 |
| WEL-17 60m×0.25mm×0.25µm | 01916-24001 |
| WEL-17 60m×0.25mm×0.5µm  | 01916-24002 |



| Specification              | P/N         |
|----------------------------|-------------|
| WEL-XE60 30m×0.25mm×0.25µm | 01917-22001 |
| WEL-XE60 30m×0.25mm×0.5µm  | 01917-22002 |
| WEL-XE60 30m×0.25mm×1.0µm  | 01917-22003 |
| WEL-XE60 50m×0.25mm×0.25µm | 01917-23001 |
| WEL-XE60 50m×0.25mm×0.5µm  | 01917-23002 |
| WEL-XE60 60m×0.25mm×0.25µm | 01917-24001 |
| WEL-XE60 60m×0.25mm×0.5µm  | 01917-24002 |
| WEL-XE60 60m×0.25mm×1.0µm  | 01917-24003 |
| WEL-XE60 30m×0.32mm×0.5µm  | 01917-32002 |
| WEL-XE60 30m×0.32mm×1.0µm  | 01917-32003 |
| WEL-XE60 50m×0.32mm×0.25µm | 01917-33001 |
| WEL-XE60 50m×0.32mm×0.5µm  | 01917-33002 |
| WEL-XE60 50m×0.32mm×1.0µm  | 01917-33003 |
| WEL-225 30m×0.25mm×0.25µm  | 01919-22001 |

| Specification             | P/N         |
|---------------------------|-------------|
| WEL-225 30m×0.25mm×0.5µm  | 01919-22002 |
| WEL-225 30m×0.25mm×1.0µm  | 01919-22003 |
| WEL-225 50m×0.25mm×0.25µm | 01919-23001 |
| WEL-225 50m×0.25mm×0.5µm  | 01919-23002 |
| WEL-225 50m×0.25mm×1.0µm  | 01919-23003 |
| WEL-225 60m×0.25mm×0.25µm | 01919-24001 |
| WEL-225 60m×0.25mm×0.5µm  | 01919-24002 |

| Specification             | P/N         |
|---------------------------|-------------|
| WEL-225 60m×0.25mm×1.0µm  | 01919-24003 |
| WEL-225 30m×0.32mm×0.25µm | 01919-32001 |
| WEL-225 30m×0.32mm×0.5µm  | 01919-32002 |
| WEL-225 30m×0.32mm×1.0µm  | 01919-32003 |
| WEL-35 30m×0.25mm×0.25mm  | 01921-22001 |
| WEL-35 30m×0.32mm×0.25µm  | 01921-32001 |
| WEL-35 30m×0.20mm×0.25mm  | 01921-12001 |

## PLOT Column

PLOT column has small granular material bonded on the pipe wall. Welch provides high quality PLOT columns which applied the unique integrated synthesis technology. Commonly used PLOT column stationary phases include styrene and its derivatives, molecular sieves and alumina, which are suitable for the separation and analysis of permanent gas and low molecular weight hydrocarbon isomers.

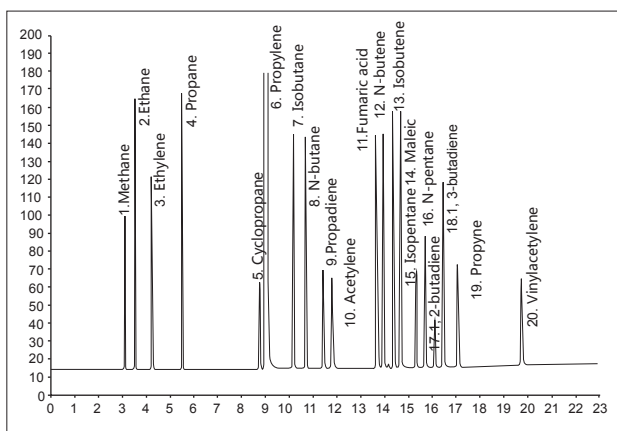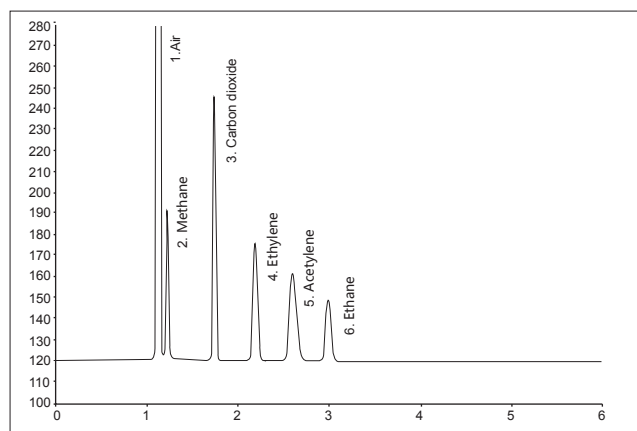

WEL-PLOT Q, 30m×0.53mm, 40µm; P/N: 06928-52026  
 Column temperature: 35 °C  
 Inlet temperature: 250 °C Detector temperature: 250 °C Detector: TCD

WEL-PLOT Al<sub>2</sub>O<sub>3</sub>, 50m×0.53mm, 25µm; P/N: 06946-53027  
 Temperature program: 80 °C (keep 5 min) → 180 °C  
 Inlet temperature: 250 °C Detector temperature: 250 °C Detector: FID

## PLOT Capillary Column

Use Alumina as the stationary phase, alumina columns can be divided into the following three kinds according to the surface treatment of alumina.

- ▶ WEL-PLOT Al<sub>2</sub>O<sub>3</sub>/KCL (Modified KCl)
- ▶ WEL-AL<sub>2</sub>O<sub>3</sub>/S (Na<sub>2</sub>SO<sub>4</sub>)
- ▶ WEL-AL<sub>2</sub>O<sub>3</sub>/M (Modified Na<sub>2</sub>MoO<sub>4</sub>)
- ▶ Polarity is similar to GS-Alumina, HP PLOT S, HP PLOT M, Alumina-PLOT, AT-Alumina, CP-Al<sub>2</sub>O<sub>3</sub>/Na<sub>2</sub>SO<sub>4</sub>

## Use divinylbenzene - polystyrene as the stationary phase

Used for analysis of alkanes, methane, air/carbon monoxide, oxides and sulfides of C1-C3 isomers, to C12.

- ▶ PLOT Q

## Use molecular sieve as the stationary phase (Carbon molecular sieve, 5A molecular sieve)

Mainly used for the detection of permanent gases, such as nitrogen, oxygen, carbon monoxide, methane and other gases.

- ▶ WEL-PLOT Molesieve

## PLOT Column Ordering Information

| Specification              | P/N         |
|----------------------------|-------------|
| WEL-PLOT Q 30m×0.32mm×20µm | 06928-32014 |
| WEL-PLOT Q 30m×0.32mm×10µm | 06928-32040 |

| Specification              | P/N         |
|----------------------------|-------------|
| WEL-PLOT Q 30m×0.53mm×20µm | 06928-52014 |
| WEL-PLOT Q 30m×0.53mm×40µm | 06928-52026 |

| Specification                                                | P/N         |
|--------------------------------------------------------------|-------------|
| WEL-PLOT Al <sub>2</sub> O <sub>3</sub> /S 50m×0.53mm×25µm   | 06951-53027 |
| WEL-PLOT Al <sub>2</sub> O <sub>3</sub> /M 50m×0.53mm×0.25µm | 06952-53001 |
| WEL-PLOT Q 30m×0.53mm×25µm                                   | 06928-52027 |
| WEL-PLOT Al <sub>2</sub> O <sub>3</sub> /S 30m×0.53mm×20µm   | 01951-52020 |

| Specification                                              | P/N         |
|------------------------------------------------------------|-------------|
| WEL-PLOT Al <sub>2</sub> O <sub>3</sub> /S 30m×0.53mm×20µm | 05951-52020 |
| WEL-PLOT Al <sub>2</sub> O <sub>3</sub> /S 50m×0.53mm×20µm | 05951-53020 |
| WEL-PLOT Al <sub>2</sub> O <sub>3</sub> /S 50m×0.32mm×8µm  | 01951-33037 |

## 1.3 Dedicated Capillary Column


For separation problem of some complex samples, Welch developed the dedicated column which can be applied to pesticide analysis, volatile organic compounds analysis, petrochemical analysis, liquor analysis and other aspects with unique performance. It requires short analysis time with good separation effect, and it is convenient for better qualitative and quantitative analysis.

| P/N         | Product                                   | Length×Inner Size×Membrane<br>m×mm×µm | Application                                           |
|-------------|-------------------------------------------|---------------------------------------|-------------------------------------------------------|
| 01929-32002 | Dedicated column A for pesticide residues | 30m×0.32mm×0.5µm                      | Organochlorine pesticide                              |
| 01929-52002 |                                           | 30m×0.53mm×0.5µm                      |                                                       |
| 01937-32002 | Dedicated column B for pesticide residues | 30m×0.32mm×0.5µm                      | Organophosphorus pesticide                            |
| 01937-52002 |                                           | 30m×0.53mm×0.5µm                      |                                                       |
| 01932-22023 | BPX-70                                    | 30m×0.25mm×0.22µm                     | Analysis of evening primrose oil                      |
| 05935-33003 | TVOC dedicated column                     | 50m×0.32mm×1.0µm                      | Total volatile organic compounds (VOCs) in indoor air |


| P/N         | Product                            | Length×Inner Size×Membrane<br>m×mm×μm | Application                               |
|-------------|------------------------------------|---------------------------------------|-------------------------------------------|
| 01936-13002 | PONA dedicated column              | 50m×0.20mm×0.5μm                      | Analysis of gasoline and diesel component |
| 01936-23002 |                                    | 50m×0.25mm×0.5μm                      |                                           |
| 05941-32002 | Dedicated column for wine analysis | 30m×0.32mm×0.5μm                      | Composition analysis of liquor and beer   |

| P/N         | Product                                   | Length×Inner Size×Membrane<br>m×mm×μm | Application                                           |
|-------------|-------------------------------------------|---------------------------------------|-------------------------------------------------------|
| 01929-32002 | Dedicated column A for pesticide residues | 30m×0.32mm×0.5μm                      | Organochlorine pesticide                              |
| 01929-52002 |                                           | 30m×0.53mm×0.5μm                      |                                                       |
| 01937-32002 | Dedicated column B for pesticide residues | 30m×0.32mm×0.5μm                      | Organophosphorus pesticide                            |
| 01937-52002 |                                           | 30m×0.53mm×0.5μm                      |                                                       |
| 01932-22023 | BPX-70                                    | 30m×0.25mm×0.22μm                     | Analysis of evening primrose oil                      |
| 05935-33003 | TVOC dedicated column                     | 50m×0.32mm×1.0μm                      | Total volatile organic compounds (VOCs) in indoor air |
| 01936-13002 | PONA dedicated column                     | 50m×0.20mm×0.5μm                      | Gasoline and diesel component analysis                |
| 01936-23002 | Dedicated column for wine analysis        | 50m×0.25mm×0.5μm                      | Composition analysis of liquor and beer               |
| 05941-32002 |                                           | 30m×0.32mm×0.5μm                      |                                                       |


### Analysis of Organochlorine Pesticide Residues

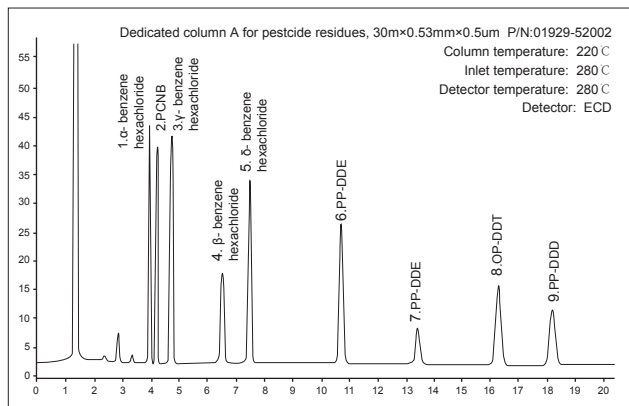


### Analysis of Liquor

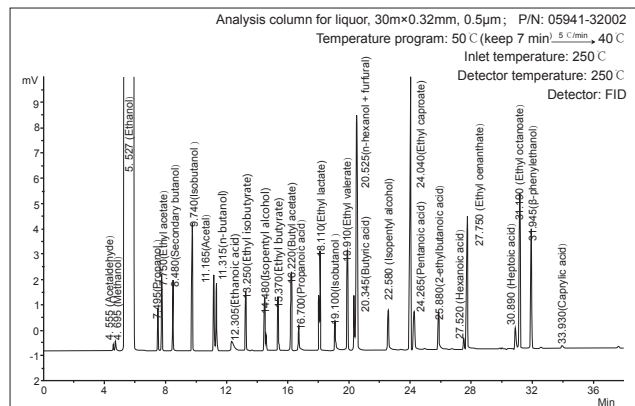

### Analysis of Liquor 2

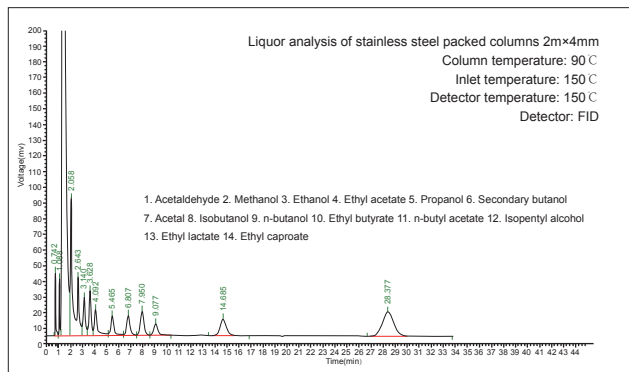

### TVOC Analysis

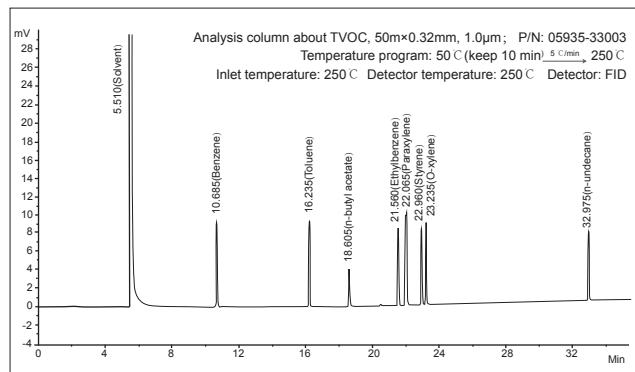

## WEL-PONA

- ▶ Dedicated column for analysis of complex hydrocarbon
- ▶ Polarity is similar to Petrocol DH, DB-Petro, HP-PONA column

### WEL-PONA Ordering Information:

| Specification             | P/N         |
|---------------------------|-------------|
| WEL-PONA, 50m×0.2mm×0.5μm | 01936-13002 |

## WM-TVOC

- ▶ Dedicated column, used for determination of total volatile organic compounds (TVOC) in indoor air

### WM-TVOC Ordering information:

| Specification              | P/N         |
|----------------------------|-------------|
| WM-TVOC, 40m×0.32mm×0.33μm | 05935-30021 |

## WM-PEG20M, WEL-PEG20M

- ▶ Polyethylene glycol column
- ▶ Bond and crosslink with strong polarity
- ▶ Recommended for fatty acids

### WM-PEG20M, WEL-PEG20M Ordering Information

| Specification               | P/N         | Specification                | P/N         |
|-----------------------------|-------------|------------------------------|-------------|
| WM-PEG20M 15m×0.2mm×0.25μm  | 05918-11001 | WM-PEG20M 50m×0.53mm×0.5μm   | 05918-53002 |
| WM-PEG20M 15m×0.2mm×0.5μm   | 05918-11002 | WM-PEG20M 60m×0.2mm×0.25μm   | 05918-14001 |
| WM-PEG20M 15m×0.25mm×0.25μm | 05918-21001 | WM-PEG20M 60m×0.2mm×0.5μm    | 05918-14002 |
| WM-PEG20M 15m×0.25mm×0.5μm  | 05918-21002 | WM-PEG20M 60m×0.25mm×0.25mm  | 05918-24001 |
| WM-PEG20M 15m×0.32mm×0.25μm | 05918-31001 | WM-PEG20M 60m×0.32mm×0.5μm   | 05918-34002 |
| WM-PEG20M 30m×0.2mm×0.25μm  | 05918-12001 | WEL-PEG20M 30m×0.25mm×0.25μm | 01918-22001 |
| WM-PEG20M 30m×0.2mm×0.5μm   | 05918-12002 | WEL-PEG20M 30m×0.25mm×0.5μm  | 01918-22002 |
| WM-PEG20M 30m×0.25mm×0.25μm | 05918-22001 | WEL-PEG20M 30m×0.25mm×1.0μm  | 01918-22003 |
| WM-PEG20M 30m×0.25mm×0.5μm  | 05918-22002 | WEL-PEG20M 50m×0.25mm×0.25μm | 01918-23001 |
| WM-PEG20M 30m×0.32mm×0.25μm | 05918-32001 | WEL-PEG20M 50m×0.25mm×0.5μm  | 01918-23002 |
| WM-PEG20M 30m×0.32mm×0.5μm  | 05918-32002 | WEL-PEG20M 50m×0.25mm×1.0μm  | 01918-23003 |
| WM-PEG20M 50m×0.2mm×0.25μm  | 05918-13001 | WEL-PEG20M 50m×0.25mm×0.4μm  | 01918-23022 |
| WM-PEG20M 50m×0.2mm×0.5μm   | 05918-13002 | WEL-PEG20M 60m×0.25mm×0.25μm | 01918-24001 |
| WM-PEG20M 50m×0.25mm×0.25μm | 05918-23001 | WEL-PEG20M 60m×0.25mm×0.5μm  | 01918-24002 |
| WM-PEG20M 50m×0.25mm×0.5μm  | 05918-23002 | WEL-PEG20M 30m×0.32mm×0.25μm | 01918-32001 |
| WM-PEG20M 50m×0.32mm×0.25μm | 05918-33001 | WEL-PEG20M 30m×0.32mm×0.5μm  | 01918-32002 |
| WM-PEG20M 50m×0.32mm×0.5μm  | 05918-33002 | WEL-PEG20M 30m×0.32mm×1.0μm  | 01918-32003 |

### Dedicated column for 37 kinds of fatty acids

| Specification              | P/N         |
|----------------------------|-------------|
| WM-CN100 100m×0.25mm×0.2μm | 07965-25011 |

**Dedicated column for liquor analysis column**

| Specification    | P/N         |
|------------------|-------------|
| 30m×0.32mm×0.5μm | 05941-32002 |

**Column pharmaceutical ethanol analysis**

| Specification    | P/N           |
|------------------|---------------|
| 30m×0.32mm×1.0μm | 05941-32003-1 |

**Dedicated column for alkyl mercury**

| Specification    | P/N         |
|------------------|-------------|
| 15m×0.53mm×0.5μm | 05971-51002 |

**Column for organic phosphorus agricultural residue**

| Specification    | P/N         |
|------------------|-------------|
| 30m×0.32mm×0.5μm | 05939-32002 |

**1.4 GC Packed Column**

**Stationary liquid:** OV-1, OV-17, OV-101, OV-225, SE-30, SE-52, SE-54, PRG-400, PEG-600, PEG-1500, PEG-4000, PEG-6000, PEG-20M, DEGS, EGA, EGS, QF-1, FFAP, DNP, β, β- Diethoxyacetonitrile, silicone oil, apiezon, squalane, DC series and etc.

**Support:** Aiatomite (Chrosorb series and others), organic support

**Adsorbent and polymer microspheres:** Porapak series, Proasil series, GDX series, HDG series, SD series, molecular sieve, carbon molecular sieve, graphitized carbon black, silica gel, aluminium oxide, etc.

**Specification:** Inner diameter 2-4 mm, length: 0.5-9 m.

◇ Welch also offers custom-made GC packed columns. Please provide GC model number, column tube type, stationary phase composition, type and particle size of the solid support, inner diameter and length, and the targeted samples.

**GC Packed Column Ordering Information:**

- | Packing Materials                  |  |
|------------------------------------|--|
| Support (e.g. Chromosorb WAW DMCS) |  |
| Mesh Number                        |  |
| Stationary Phase A                 |  |
| Stationary Phase A Coated Amount/% |  |
| Stationary Phase B                 |  |
| Stationary Phase B Coated Amount/% |  |
- |                |                                                                                                                                                         |
|----------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
| Tube materials | <input type="checkbox"/> Stainless Steel <input type="checkbox"/> Passivated stainless steel <input type="checkbox"/> Glass <input type="checkbox"/> PP |
|----------------|---------------------------------------------------------------------------------------------------------------------------------------------------------|
- |                                                        |  |
|--------------------------------------------------------|--|
| Instrument Model (e.g. Agilent 7890A/ Shimadzu 2014 C) |  |
|--------------------------------------------------------|--|
- | Dimension          | Note                                                  |
|--------------------|-------------------------------------------------------|
| Length/m           |                                                       |
| OD/mm              | For Stainless Steel GC packed column, OD is required. |
| ID/mm              | For glass packed column, ID is required               |
| Center Distance/mm | For glass packed column, Center distance is required  |

Note:

Before ordering a packed column, first verify that the GAS chromatograph instrument has a column inlet for injecting.

When ordering stainless steel packed column, please provide the instrument type and the outer diameter of the packed column.

When ordering glass packed column, please provide the instrument type and the center distance between the injector and the detector.


**Application of GC Column****2.1 Application of GC Column in Chemical Energy Field****Analysis of high carbon fatty acid methyl ester by high temperature resistant crosslinked polar column**

**Characteristics:** The high carbon fatty acid methyl ester can be analyzed to solve the difficulty of high temperature resistance of polar column. The maximum temperature of modified column can reach 320°C.


## Analysis of Biodiesel on High-carbon Fatty Acid Methyl Ester Column

**Characteristics:** The high carbon fatty acid methyl ester in biodiesel was analyzed to solve the difficulty of high temperature resistance of polar column. The maximum temperature of modified column could reach 320°C.

### High Temperature Resistant Crosslinked Polar Column

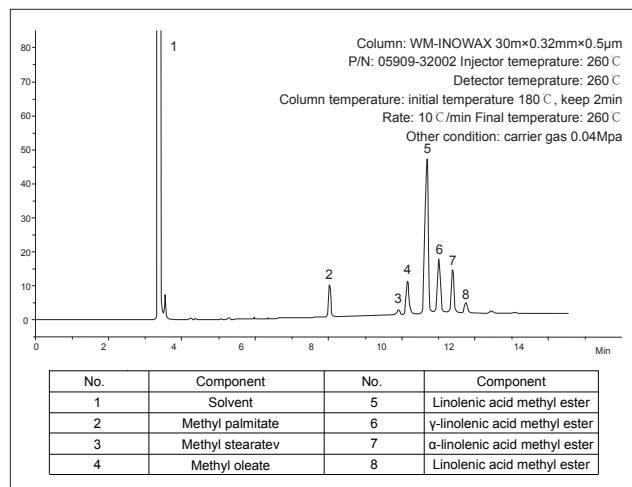



### High-carbon Fatty Acid Methyl Ester Column

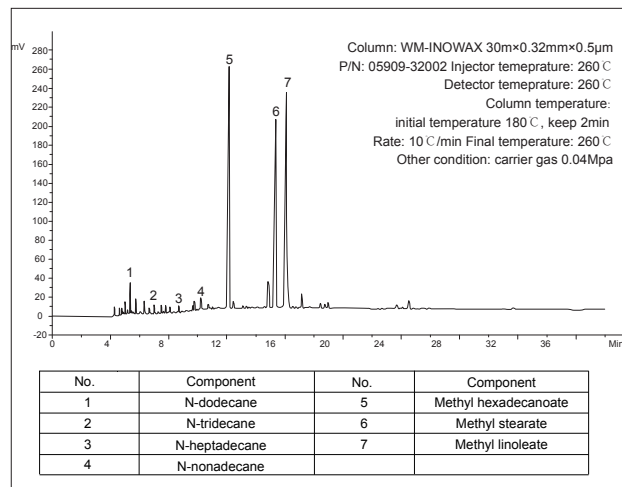

## Analysis of Oxidation and Aromatics in Gasoline


**Characteristics:** comply with SH/T 0663 analysis requirements for alcohols and ethers in gasoline

**Characteristics:** comply with SH/T 0693 aromatics analysis requirements in gasoline

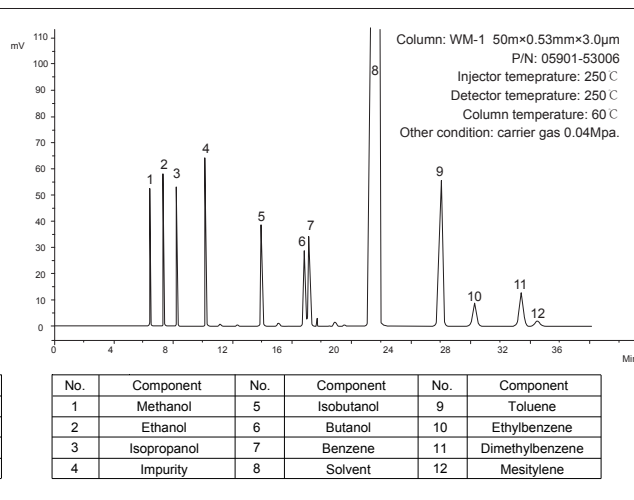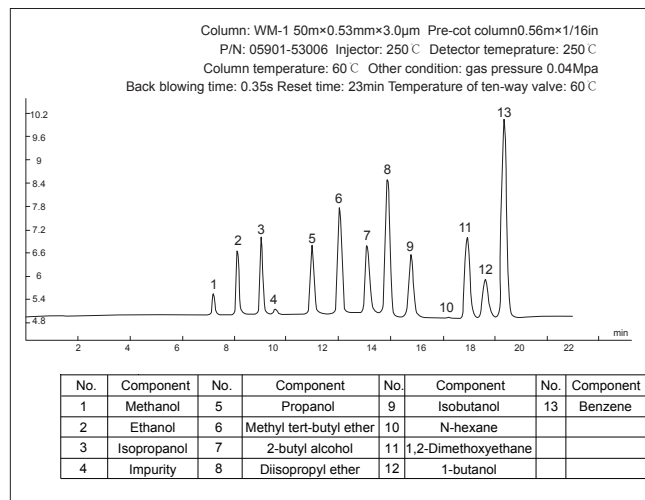


## Chromatogram of Pyrolysis Gas Group Analyzed by Capillary Column

**Characteristics:** analyze C1-C7, the olefins are effectively separated from the olefins

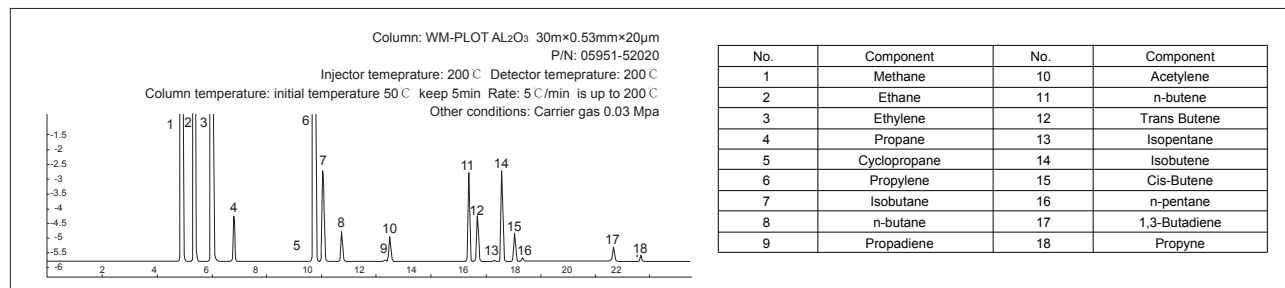


## Analyze Industrial Phenols by Dedicated Column

**Characteristics:** analyze the components of phenolic products

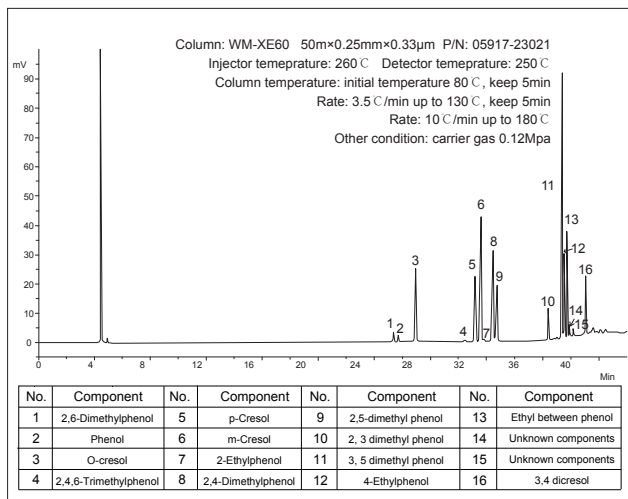


## Analyze Purity of P-methoxyphenol by Phenolic Dedicated Column


**Characteristics:** analyze purity of p-methyl phenol, and achieve baseline separation of o-methyl phenol, p-methyl phenol and m-methyl phenol.

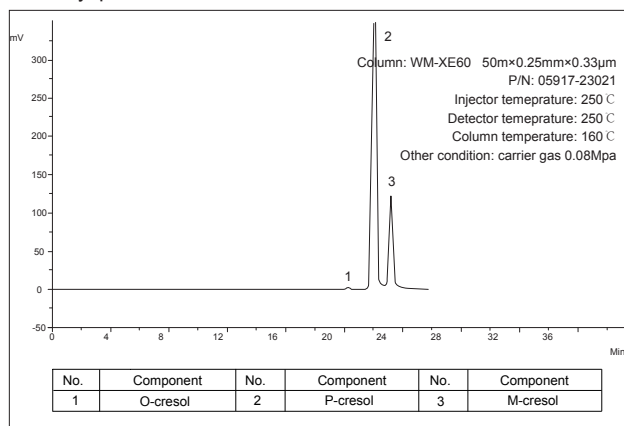

## Analyze Refrigerant R22 by Dedicated column

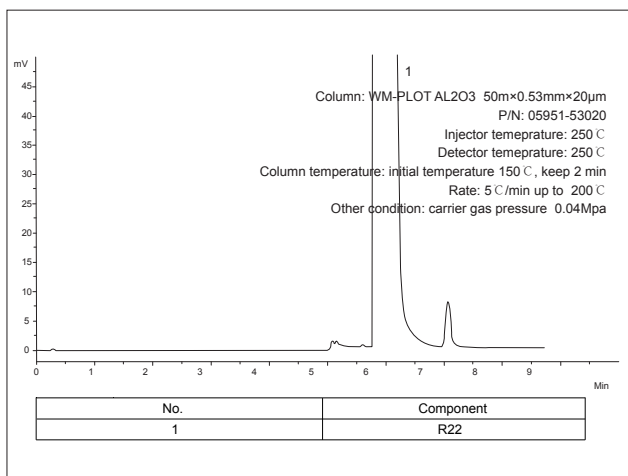


## Analyze Mixed Gas Refrigerant by Dedicated Column

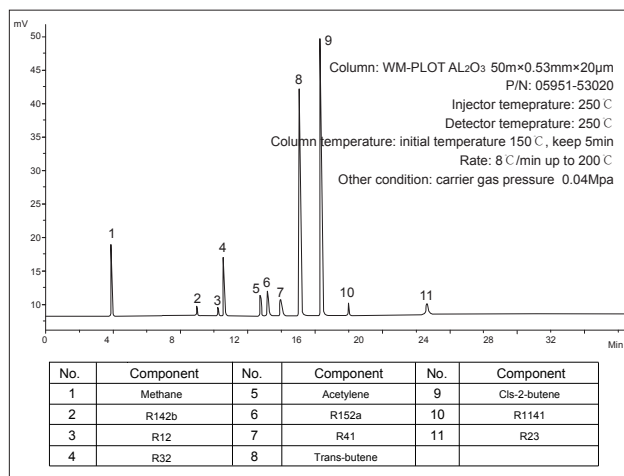


## Analyze Cyclohexane and Benzene

**Characteristics:** effectively analyze of cyclohexane and benzene. It can be used to detect benzene or benzene in cyclohexane cyclohexane

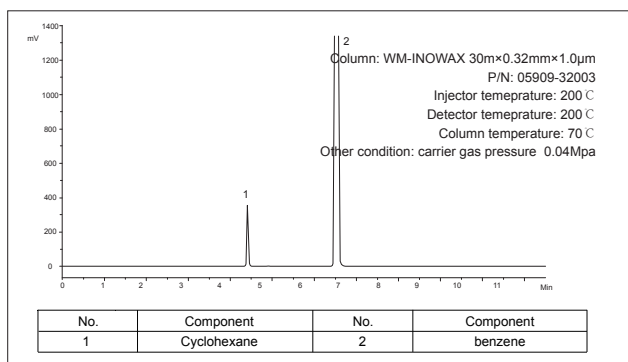


## Analyze Purity of p-phthalic Anhydride by Dedicated Column in Chromatographic Way

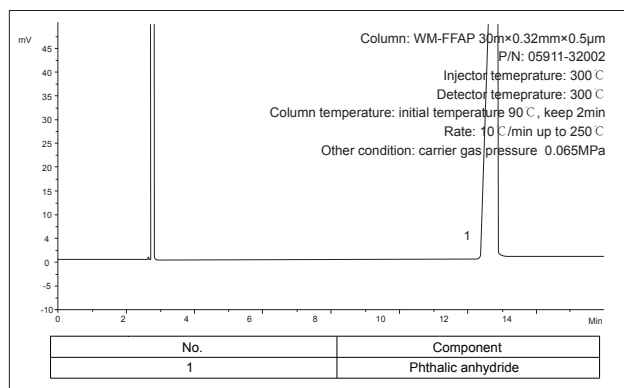




## Analyze Chloroethane Purity by Capillary Column

**Characteristics:** analyze purity of chloroethane and the content of ethanol in chloroethane by capillary column

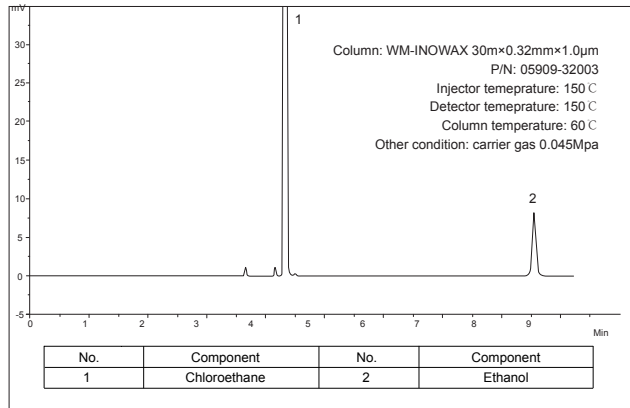

## Analyze methanol purity by Capillary Column

**Characteristics:** if use capillary column to analyze the trace alcohol and related impurities in methanol, the methanol tailing would improve with good separation effect.

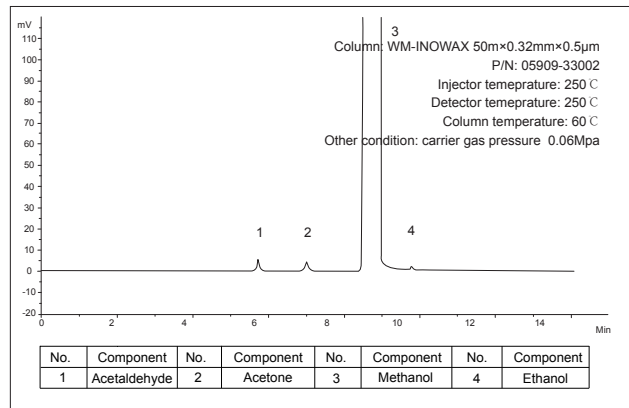


## 2.2 Application of GC Column in Brewing Field

**Characteristics:** in addition to alcohols and esters, organic acids, such as acetic acid, butyric acid and pentanoic acid can be well analyzed according to temperature programming. Baseline separation of methanol, acetaldehyde, ethanol and ethyl acetate can be achieved for temperature-programmed analysis of more components. More components also can be analyzed by temperature programming.

### Liquor Capillary Column C1

C1 column can be used to analyze various mixed components of liquor, and there are up to 30 qualitative components at present.

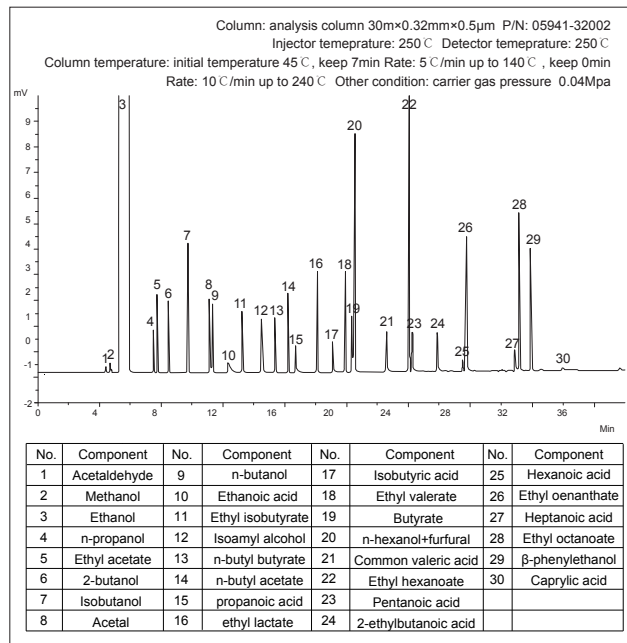


### Analyze with Large Diameter Dediacted Column for Liquor



**Characteristics:** can be used for thermostatic analysis and completely separate methanol, acetaldehyde, ethyl acetate.

### Liquor capillary column C2

C2 column has been upgraded on the basis of Liquor analysis C1 column, which can analyze more components such as 3-methiopropyl alcohol, n-hexanol, etc. Suitable for separation of acids. At present, there are 36 qualitative components

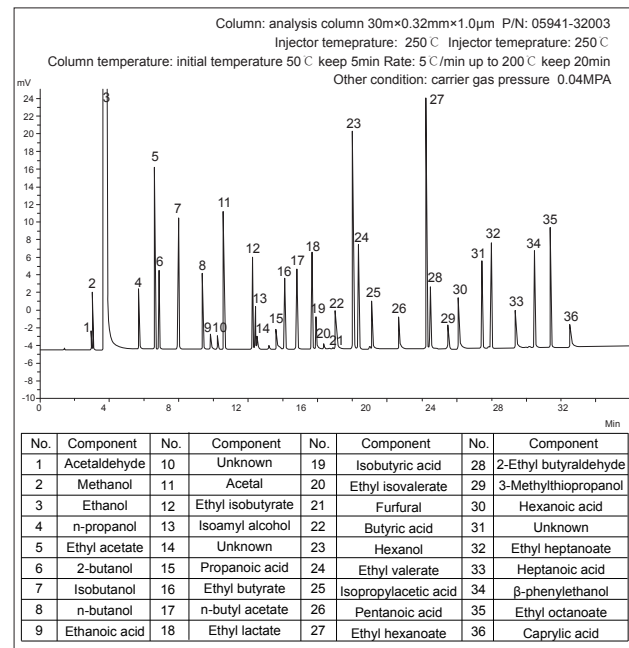


### Constant temperature analysis of by Small Diameter Dediacted Column for Liquor

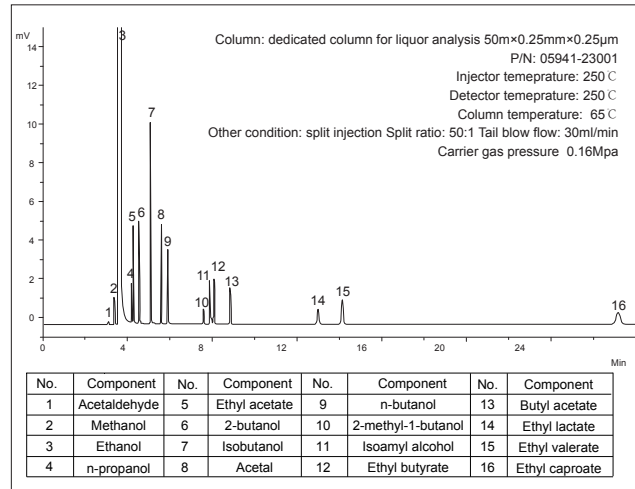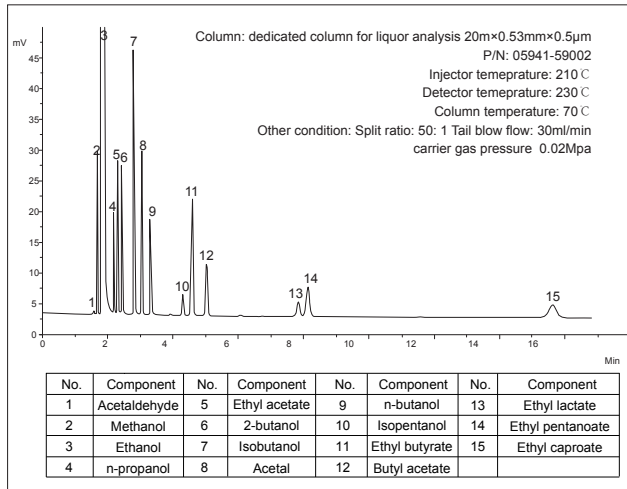

## Analyze the Content of β-phenylethanol in Black Rice Wine


**Characteristics:** determine β-phenylethanol in black rice wine with 2-ethyln-butyric acid as internal standard. This method can also be used for the analysis of other similar yellow rice wine products

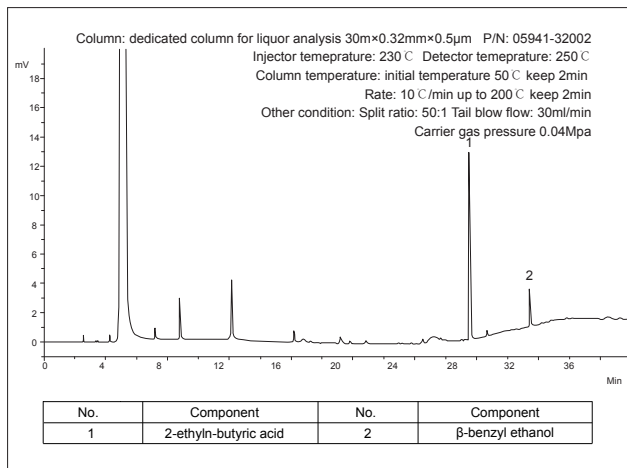

## 2.3 Application of GC Columns in Environmental Analysis


Separation of benzene series samples by capillary column

**Characteristics:** analyze eight kinds of benzene series samples

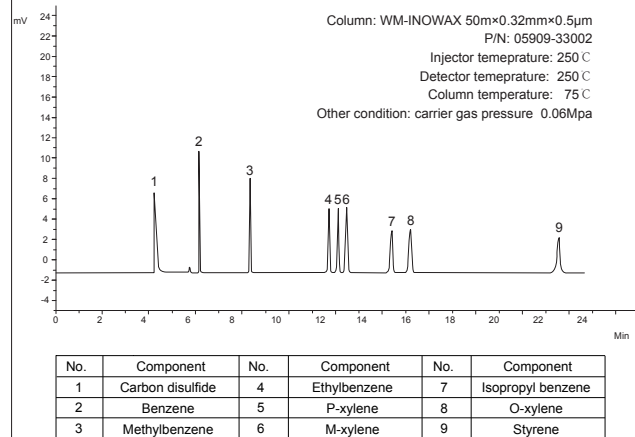


## Analyze the Benzene Series Samples by High Temperature Resistant Capillary Column

**Characteristics:** comply with HJ 583/584 standards, analyze the maximum temperature of 8 benzene series samples up to 320 C, more durable than normal benzene column.

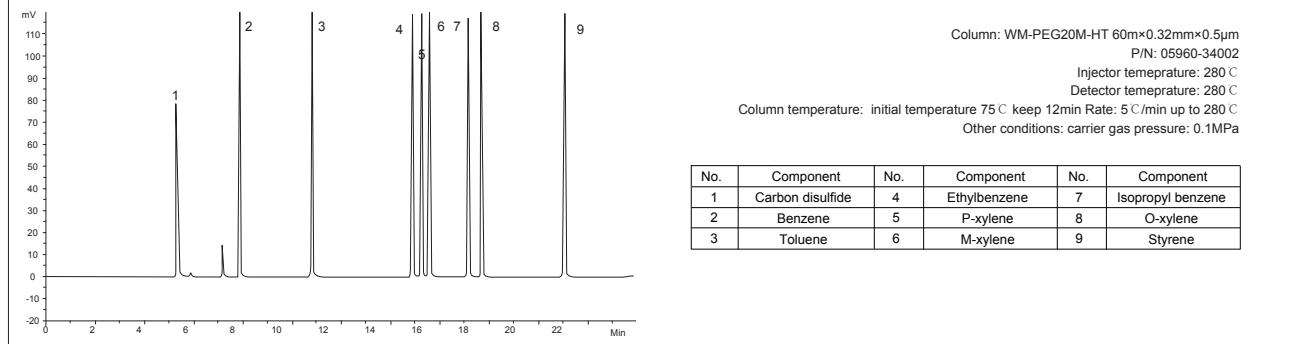


## TVOC Column for Rapid Analysis

**Characteristics:** 8 kinds of volatile toxic and harmful substances in the indoor environment can achieve baseline separation within 10 min.

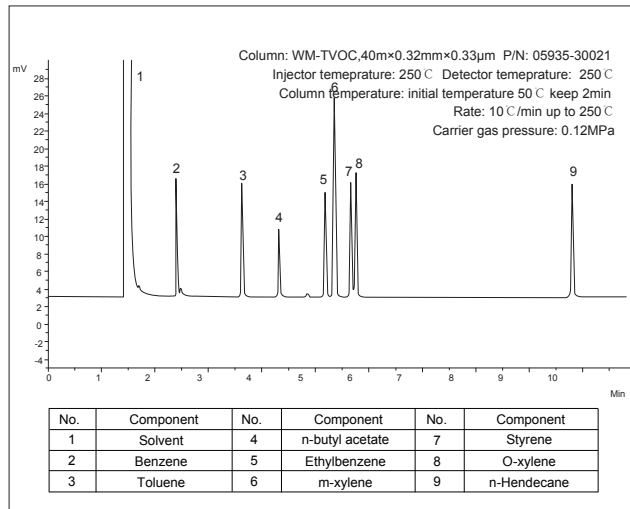


## TVOC Special Capillary Column for Portable Micrometer

**Characteristics:** it can be used for portable miniature TVOC detector, which has the advantages of fast speed, good efficiency and convenient analytical conditions, etc., and is specially customized for miniature chromatograph

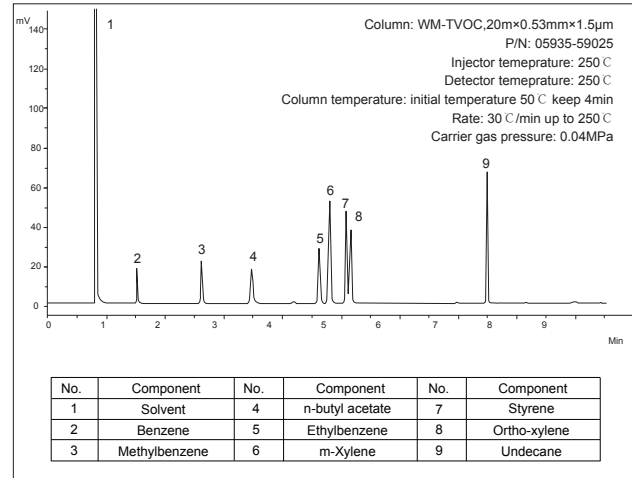

## Residue Analysis of Styrene


**Characteristics:** analyze the residue of styrene in polystyrene

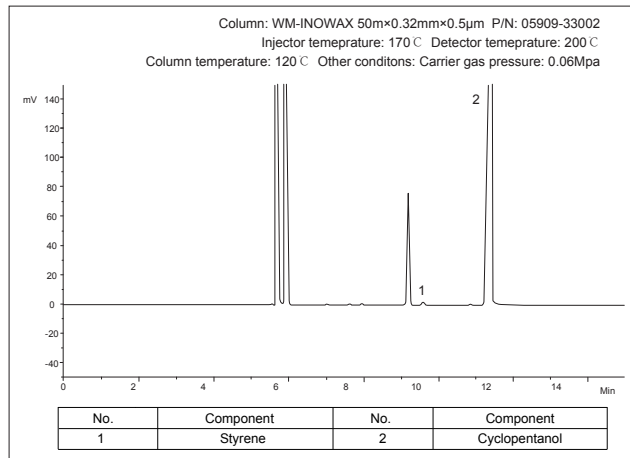

## 2.4 Application of GC column in Food Field


### DHA, EPA Analysis

**Characteristics:** determine the content of DHA and EPA in fish oil by GC capillary column

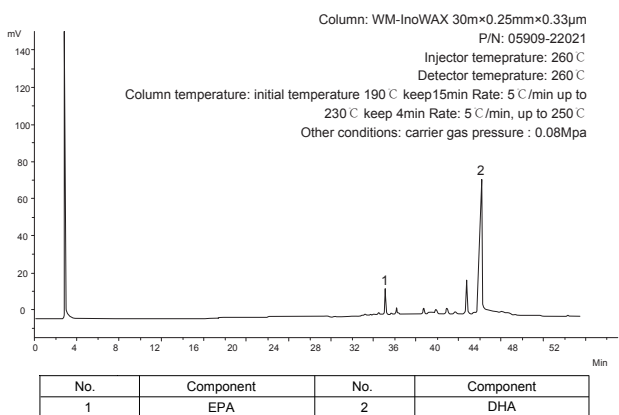


### Analyze Fatty Acid Component

**Characteristics:** select GC capillary column to detect fatty acid components with good separation effect. The maximum temperature of the column can be up to 320 C

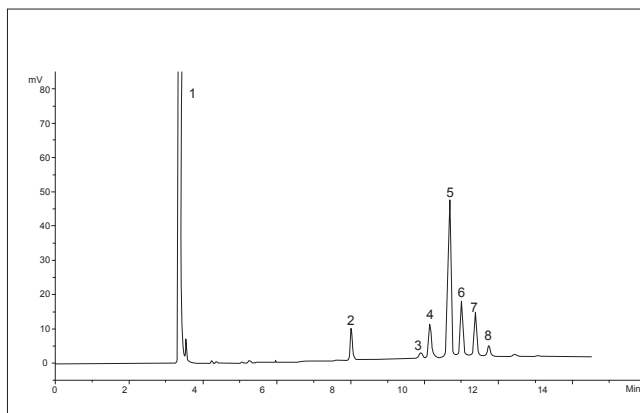


## Analysis of Organophosphorus Pesticide Residues in Food

**Characteristics:** according to the pharmacopoeia, the content of menthol and camphor was detected by the capillary column

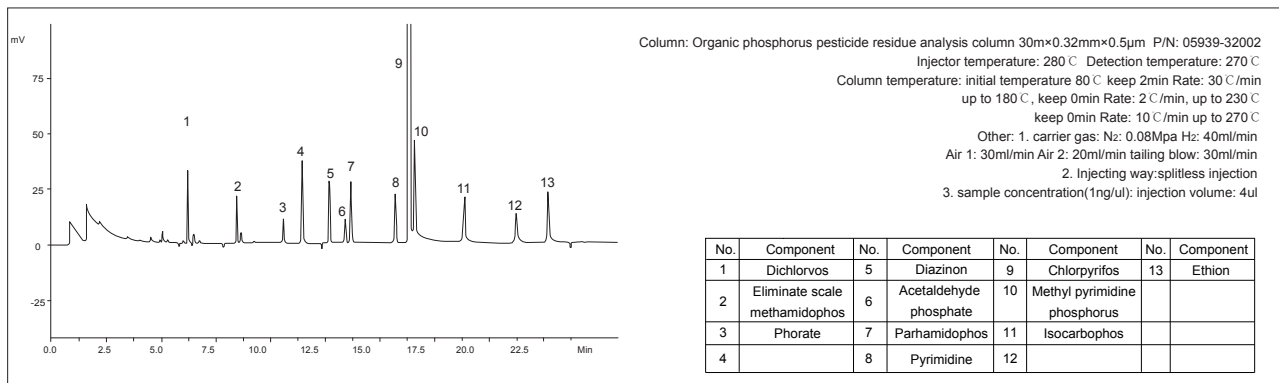


## Analysis of Organochlorine Pesticide Residues in Food

**Characteristics:** constant temperature analysis of capillary column to achieve baseline separation benzene hexachloridex and DDT eight components

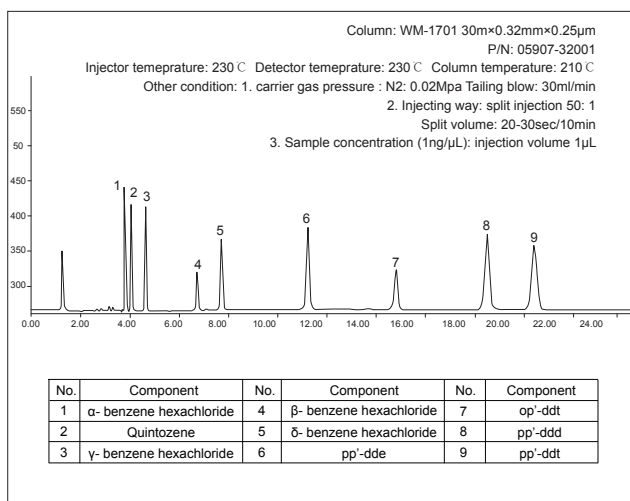


## Chromatogram Analysis of C1-C6 Organic Acids


**Characteristics:** constant temperature analysis of capillary column to achieve baseline separation benzene hexachloridex and DDT eight components

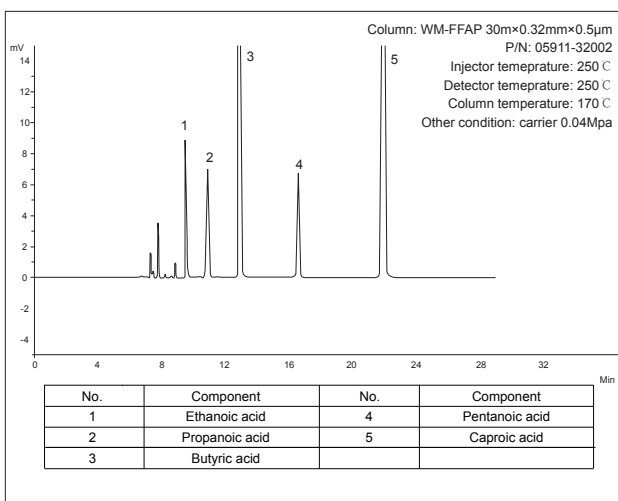

## Analysis of Formaldehyde, Methyl acetal, Methyl formate, Methanol and Methyl orthoformate

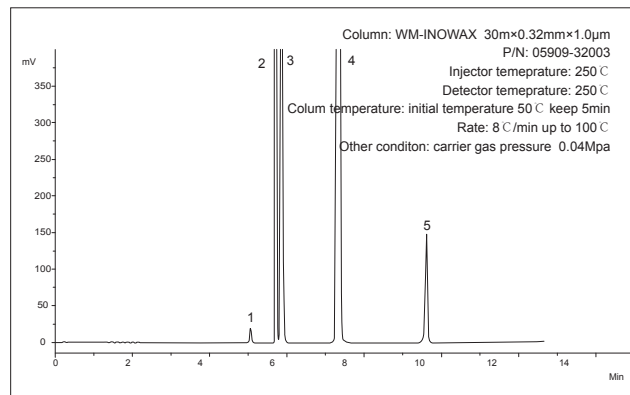

## Analysis of n-Methylpyrazine Residue

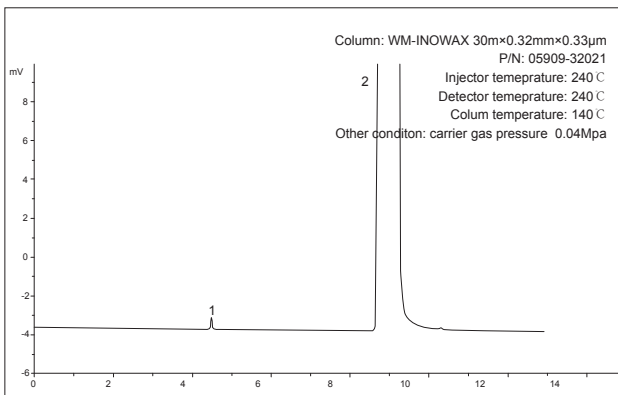

| No. | Component      | No. | Component              |
|-----|----------------|-----|------------------------|
| 1   | Formaldehyde   | 4   | Methanol               |
| 2   | Methylal       | 5   | Trimethyl orthoformate |
| 3   | Methyl formate |     |                        |


| No. | Component        | No. | Component          |
|-----|------------------|-----|--------------------|
| 1   | n-methylpyrazine | 2   | Dimethyl sulfoxide |

## 2.5 Application of GC Column in Pharmacopoeia


According to the provisions of the 2020 edition of Chinese Pharmacopoeia and the actual needs of customers, Welch specially launched the pharmacopoeia GC detection chromatogram atlas. Welch GC column perfectly conforms to the pharmacopoeia's requirements for column effect, resolution and tailing factor, etc., with good quality stability and excellent inter-batch reproducibility, which provides a strong guarantee for pharmaceutical enterprises to monitor drug quality.

### Analysis of Tropine Mixed Samples

**Characteristics:** analyze the reactants of tropine in medicine

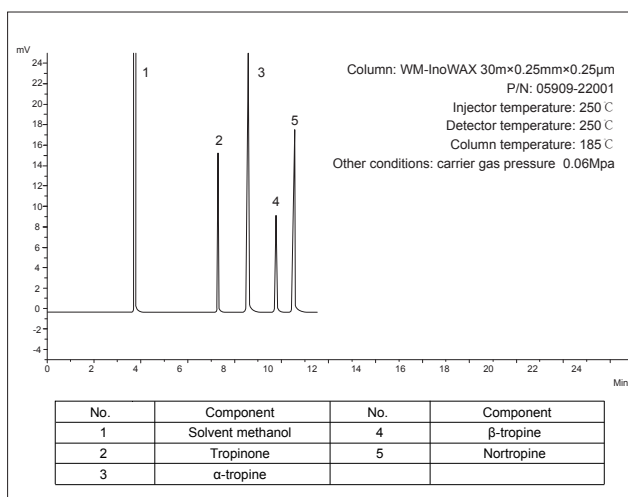


### Analysis of the Purity of Nortropine

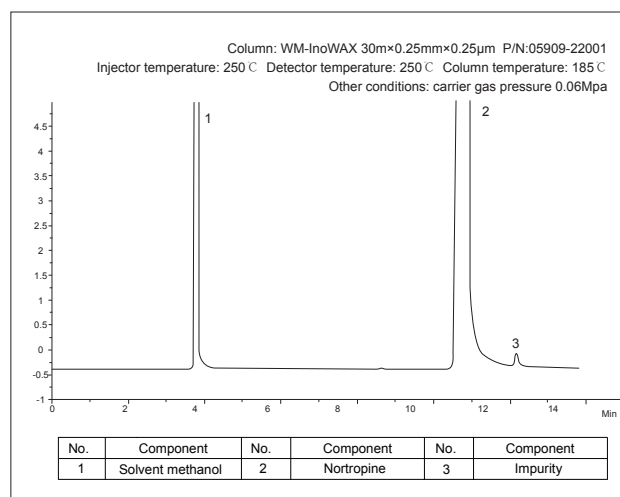


### Analysis of Chloroethanol in Water

**Characteristics:** analyze the 2-chlorine ethanol residue in medical devices or hollow capsules in accordance with the pharmacopoeia, use water as solvent for direct injection analysis

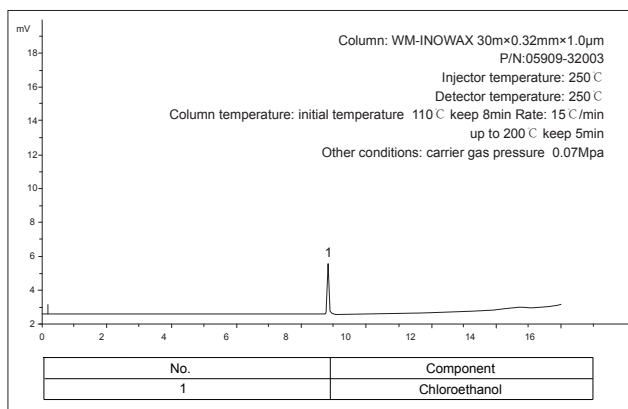


### Analysis of Ethylene Oxide

**Characteristics:** Use headspace injection to analyze ethylene oxide residue in medical devices or hollow capsules. The column can also be used for 2-chloroethanol analysis

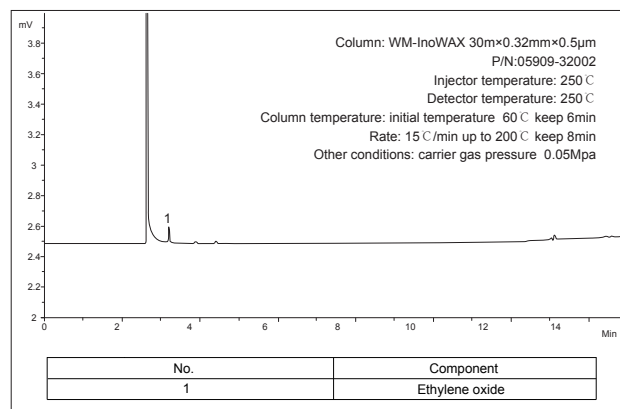


### Analysis of Borneol Capillary Column 1

**Characteristics:** referring to the analysis requirements of natural borneol and synthetic borneol in the pharmacopoeia, select the capillary column specified in the pharmacopoeia to detect the content of isoborneol and borneol in borneol, and the analysis effect was better than that of packed column

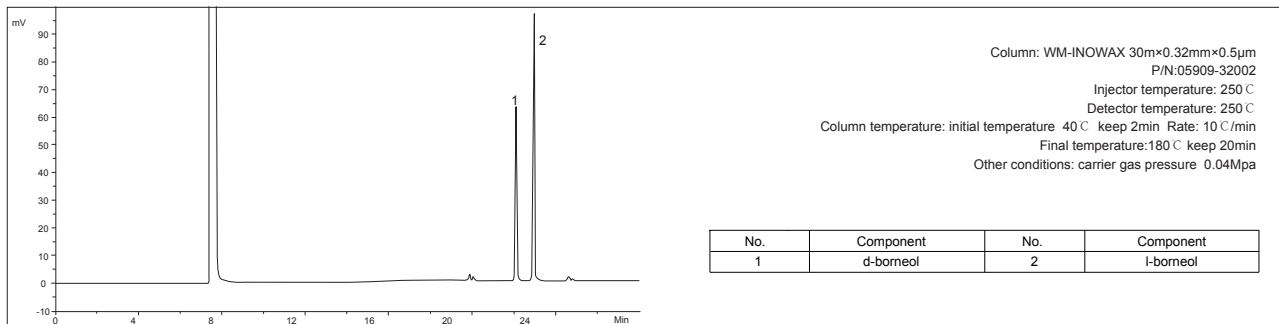


### Analysis of Borneol by Capillary Column 1

**Characteristics:** to determine the contents of isobornol and borneol in borneol by capillary column, because this column has better analysis effect of the than that of the packed column and faster analysis speed than that of borneol capillary column 1

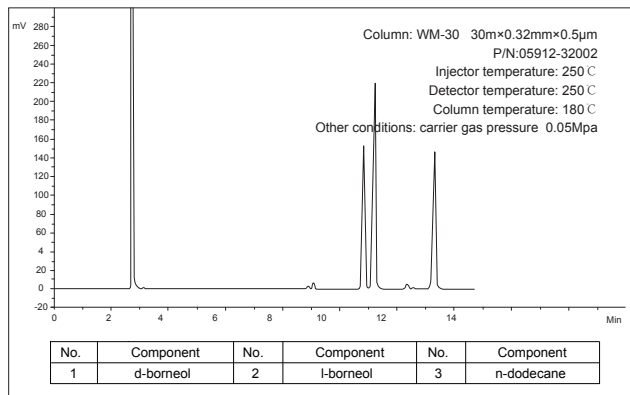


### Analysis of Camphor, Camphor and Safrol in Essential Oil

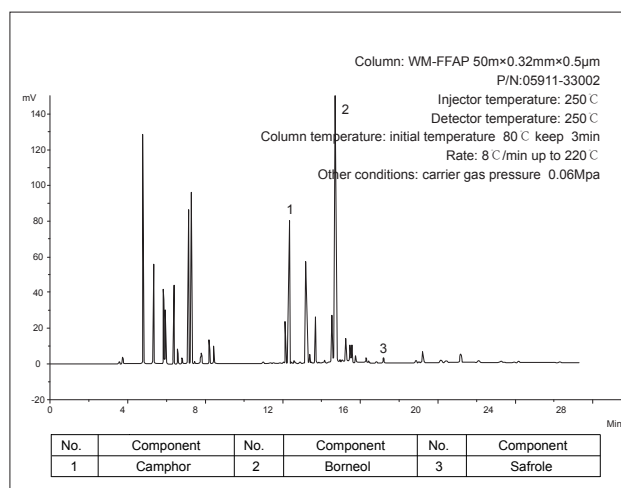


### Analysis of Coarse Morpholine

**Characteristics:** the capillary column is suitable for detecting the purity of morpholine raw material and the composition of morpholine treated with dehydrogenation

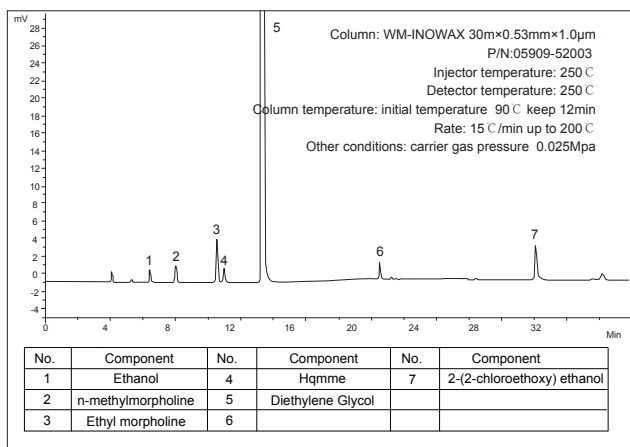


### Analysis of Morpholine

**Characteristics:** The column can be used for analysis of related components of morpholine with good reproducibility and high resolution

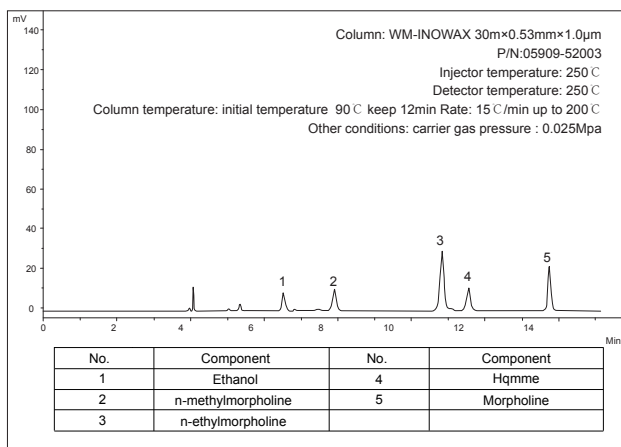


### Determination of Ethanol Volatile Substance

**Characteristics:** according to the determination method requirements of volatile substances in the pharmacopoeia, select capillary column to test the purity of ethanol

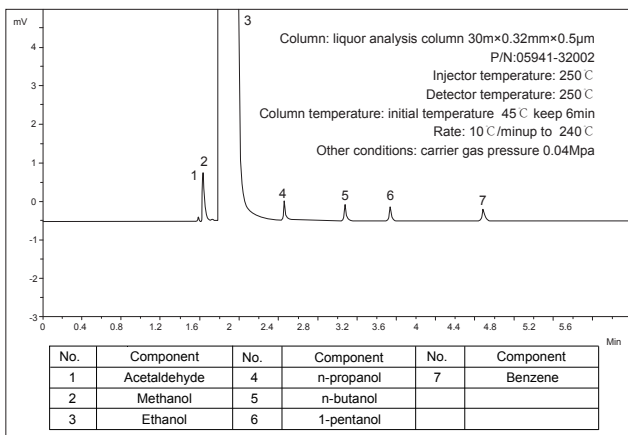


### Analysis of Plasticizer

**Characteristics:** this capillary column is suitable for detecting the components of phthalate plasticizer in medical packaging

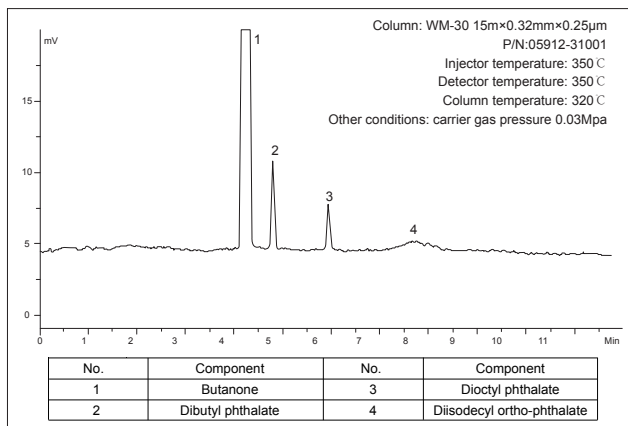


### Analysis of Menthol Camphor

**Characteristics:** according to the pharmacopoeia, use the capillary column to detect menthol camphor content

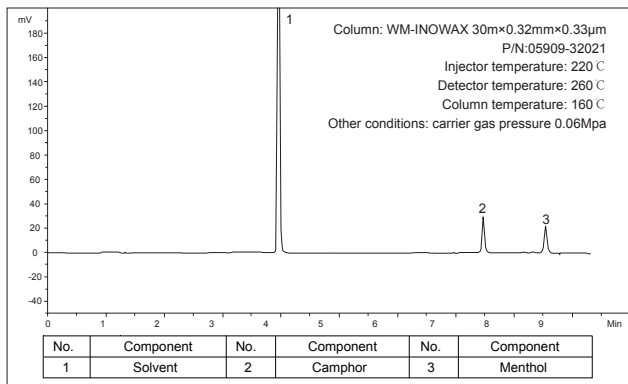


### Analysis of Maleic Anhydride and Succinic Anhydride

**Characteristics:** the capillary column is suitable for the detection of maleic anhydride and succinic anhydride with high analytical accuracy and symmetry peak

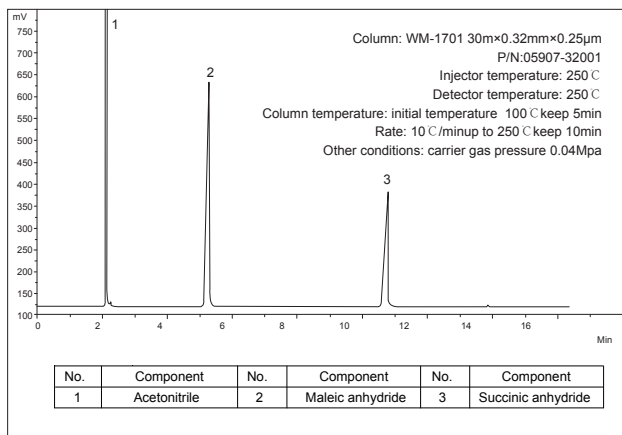


### Analysis of Magnesium Stearate


**Characteristics:** according to the requirement of magnesium stearate analysis in the pharmacopoeia, convert the magnesium stearate into methyl stearate by capillary column

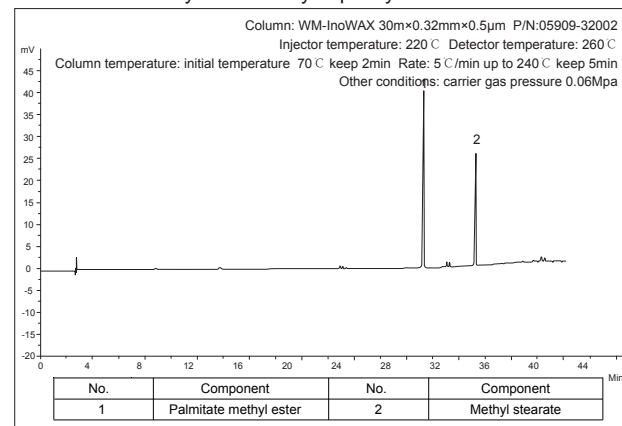


### Separation of Acetic Acid and Acetic Anhydride by Capillary Column

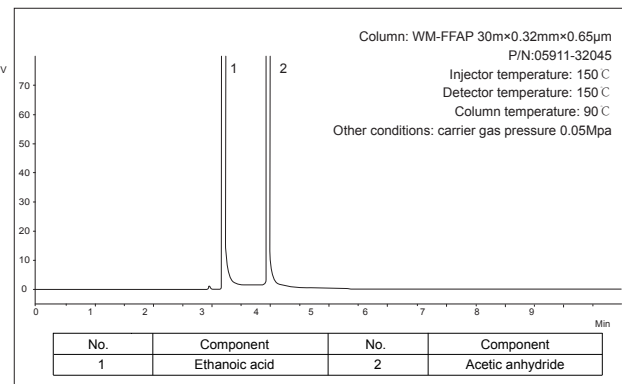


## Amomum

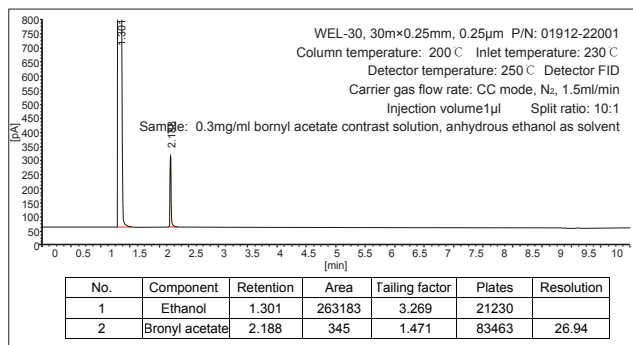



## Pogostemon Cablin

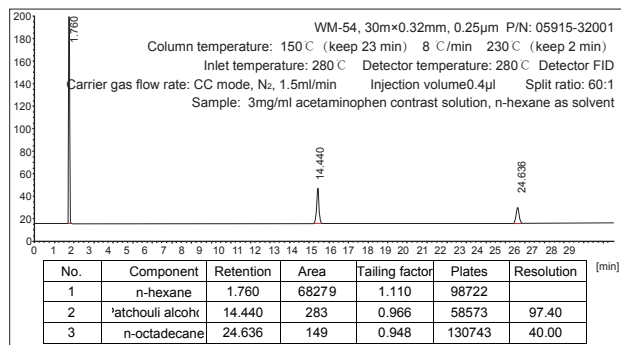


## Fructus Anisi Stellati

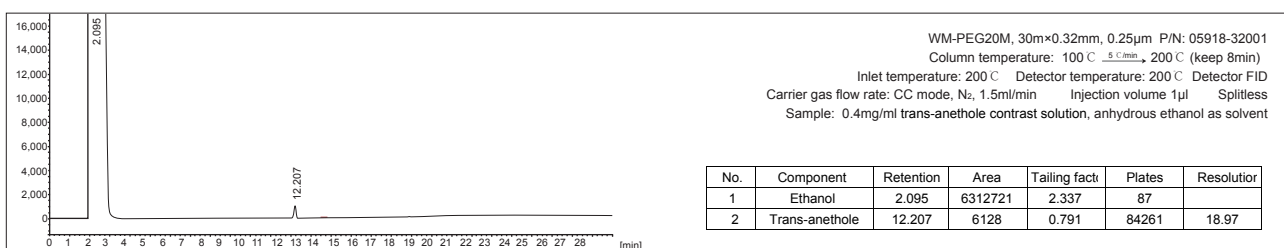


## Pine Nodular Branch

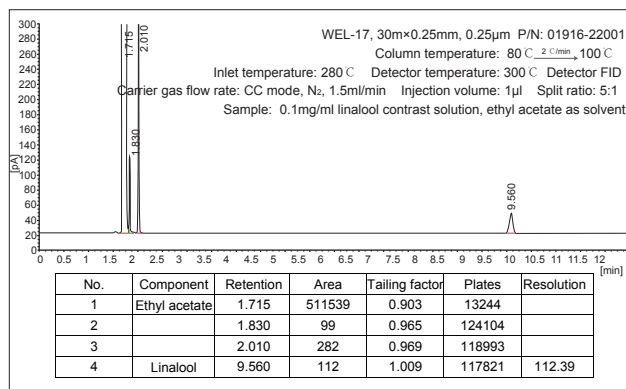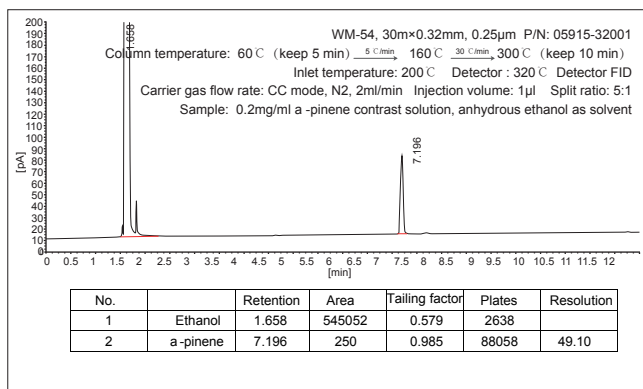

## Fennel

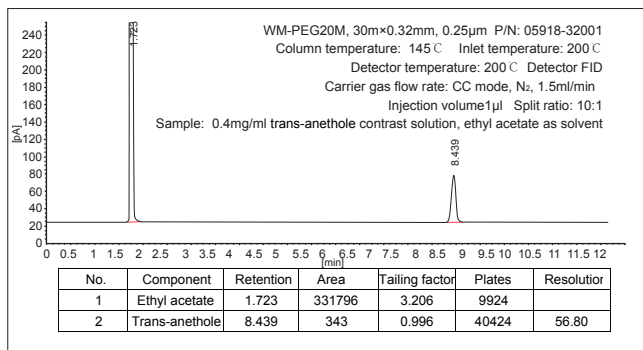


## Elecampane

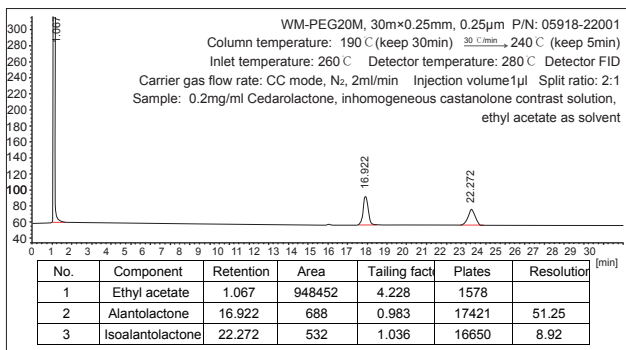






## Frankincense Somalia

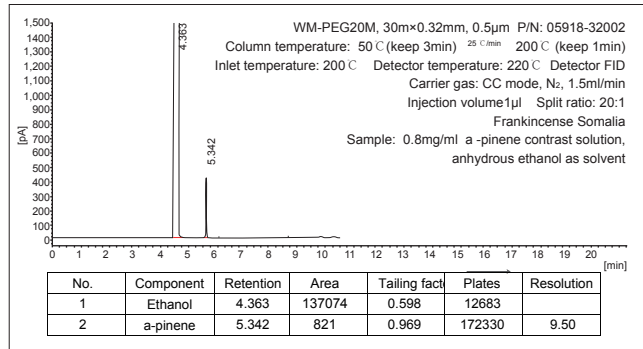


## Ethiopian Frankincense

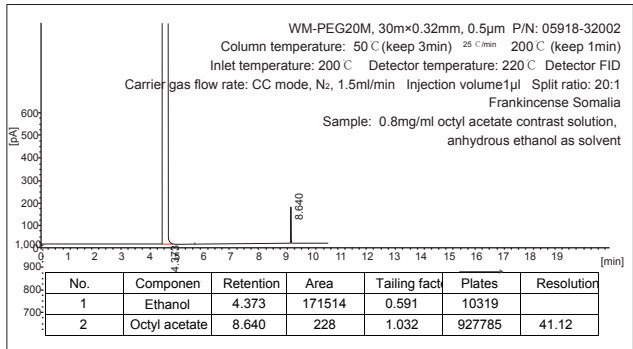


## Moschus

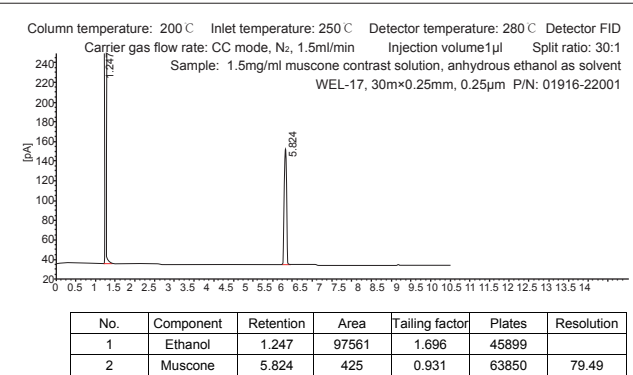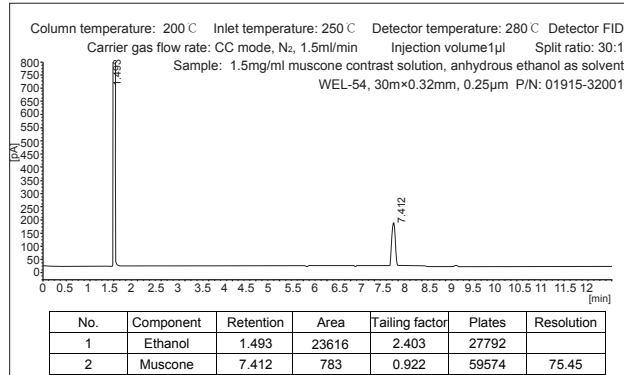


## Menthol

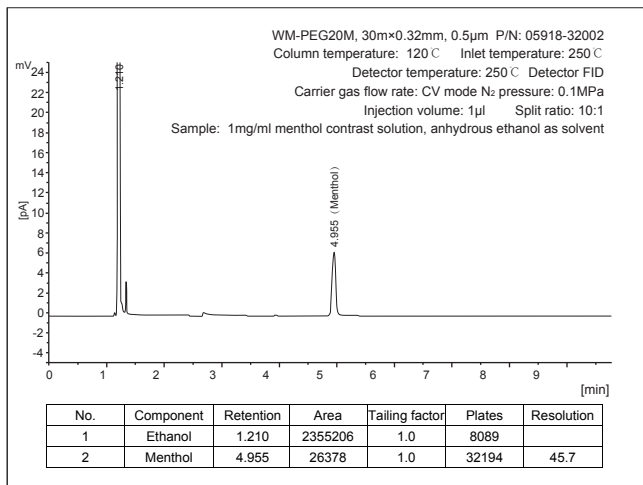


## Cloves

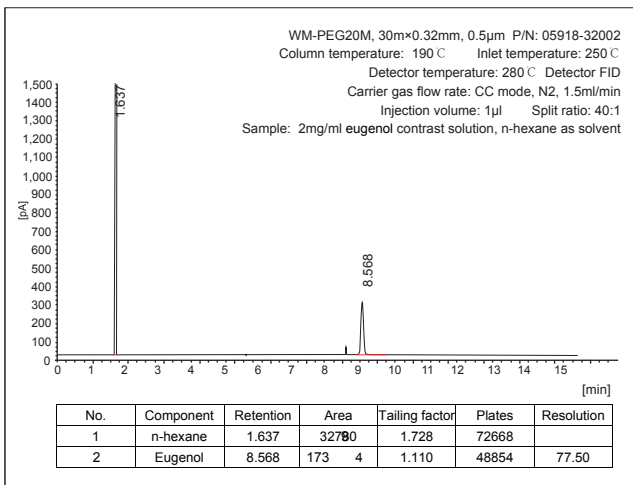

## Folium Artemisiae Argyi

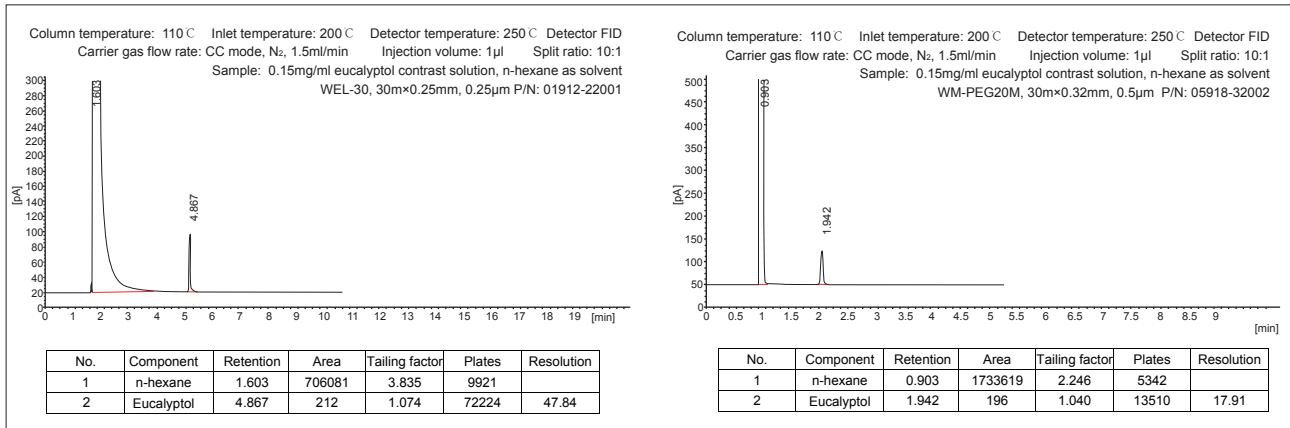


## Nutmeg

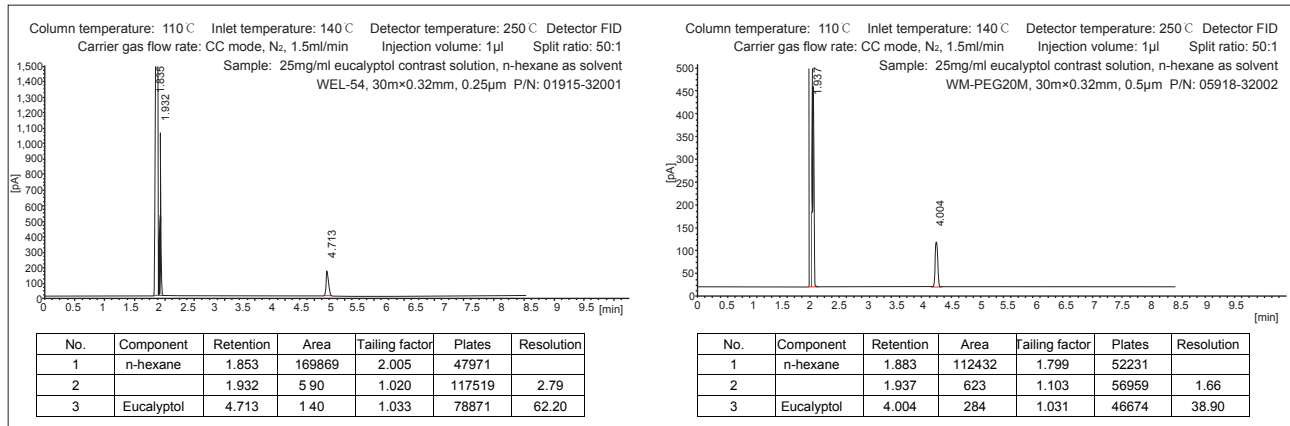


## 2.6 Other Applications of GC Columns


### Amoxicillin Residual Solvent

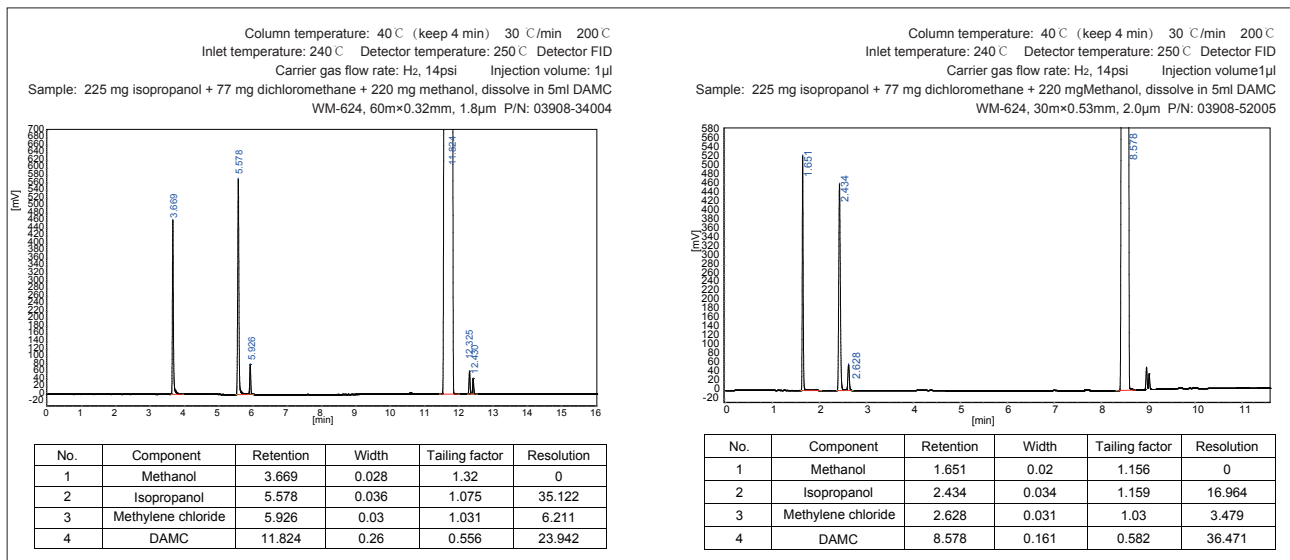

## Solvent Separation

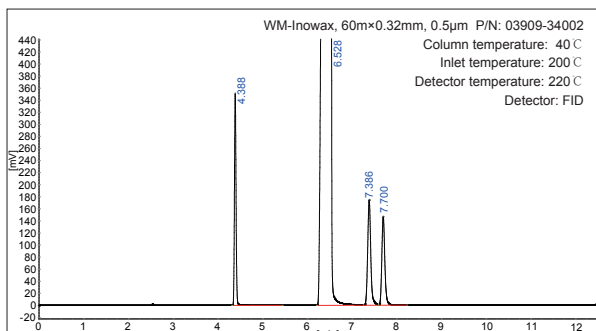


| No. | Component   | Retention | Half width | Tailing factor | Resolution |
|-----|-------------|-----------|------------|----------------|------------|
| 1   | Acetone     | 4.388     | 0.036      | 1.1            | 0          |
| 2   | Methanol    | 6.528     | 0.226      | 0.564          | 9.611      |
| 3   | Isopropanol | 7.386     | 0.067      | 1.14           | 3.445      |
| 4   | Ethanol     | 7.7       | 0.066      | 1.185          | 2.787      |

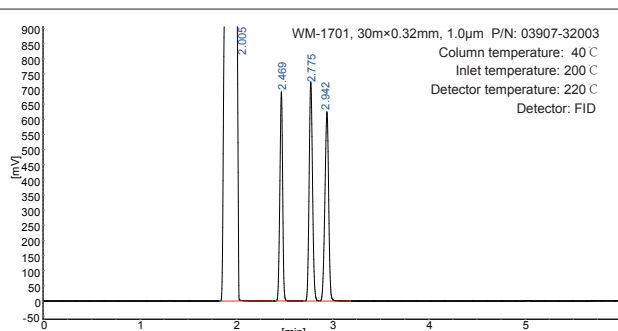


| No. | Component   | Retention | Half width | Tailing factor | Resolution |
|-----|-------------|-----------|------------|----------------|------------|
| 1   | Methanol    | 2.005     | 0.145      | 0.559          | 0          |
| 2   | Ethanol     | 2.469     | 0.029      | 0.929          | 3.135      |
| 3   | Acetone     | 2.775     | 0.035      | 1.069          | 5.55       |
| 4   | Isopropanol | 2.942     | 0.039      | 0.943          | 2.625      |

## Related Substance of Propanediol

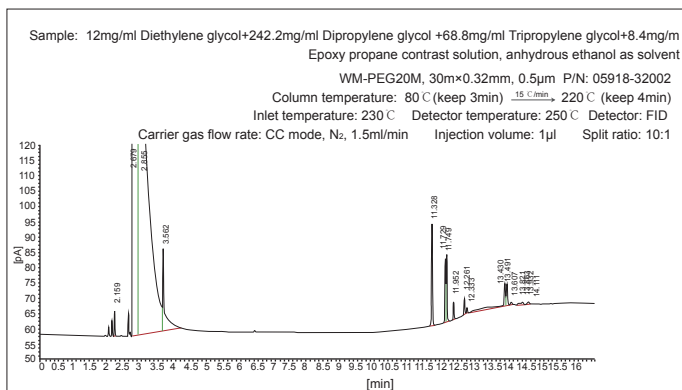


| No. | Component           | Retention | Area     | Tailing factor | Plates  | Resolution |
|-----|---------------------|-----------|----------|----------------|---------|------------|
| 1   | Propylene oxide     | 2.159     | 8.7      | 1.148          | 98077   | 2.63       |
| 2   | Anhydrous ethanol   | 2.679     | 613153.3 | 4.373          | 11402   | 1.09       |
| 3   | Anhydrous ethanol   | 2.855     | 2025.5   | 7.041          | 1086    | 0.79       |
| 4   | Impurity            | 3.562     | 124.8    | 3.782          | 57734   | 3.49       |
| 5   | Dipropylene glycol  | 11.328    | 62.5     | 1.016          | 833078  | 103.00     |
| 6   | Dipropylene glycol  | 11.712    | 37.6     | 1.056          | 992838  | 7.97       |
| 7   | Dipropylene glycol  | 11.749    | 40.9     | 0.999          | 891837  | 0.78       |
| 8   | Dipropylene glycol  | 11.952    | 10.5     | 1.027          | 938722  | 4.10       |
| 9   | Dipropylene glycol  | 12.261    | 9.9      | 1.065          | 1020006 | 6.33       |
| 10  | Diethylene glycol   | 12.333    | 3.5      | 0.945          | 1045708 | 1.50       |
| 11  | Tripropylene glycol | 13.430    | 44.9     | 0.528          | 506934  | 17.78      |
| 12  | Tripropylene glycol | 13.491    | 19.8     | 1.052          | 512213  | 0.81       |
| 13  | Tripropylene glycol | 13.607    | 3.8      | 1.027          | 279177  | 1.30       |
| 14  | Tripropylene glycol | 13.821    | 1.2      | 0.941          | 651177  | 2.50       |
| 15  | Tripropylene glycol | 13.863    | 1.1      | 1.046          | 778881  | 0.64       |
| 16  | Tripropylene glycol | 13.932    | 2.6      | 0.832          | 402300  | 0.93       |
| 17  | Tripropylene glycol | 14.110    | 2.3      | 0.988          | 577699  | 2.20       |

## Content of propanediol

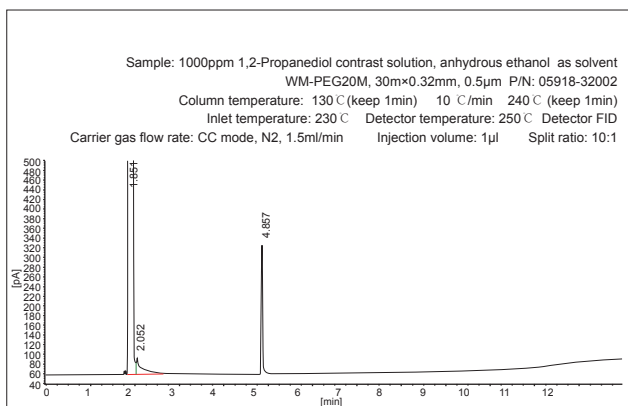

| No. | Component   | Retention | Area   | Tailing factor | Plates | Resolution |
|-----|-------------|-----------|--------|----------------|--------|------------|
| 1   | Ethanol     | 1.851     | 477568 | 4.413          | 5583   | 0          |
| 2   | Impurity 1  | 2.052     | 302    | 6.579          | 4496   | 1.82       |
| 3   | Propanediol | 4.857     | 539    | 1.195          | 153604 | 32.71      |


## Methoxy, ethoxy

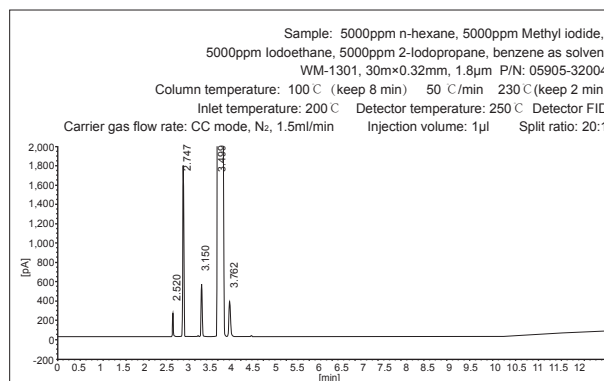

| No. | Component     | Retention | Area   | Tailing factor | Plates | Resolution |
|-----|---------------|-----------|--------|----------------|--------|------------|
| 1   | Methyl iodide | 2.520     | 297    | 1.039          | 95973  | 0          |
| 2   | n-hexane      | 2.747     | 2674   | 1.043          | 75243  | 6.28       |
| 3   | Iodoethane    | 3.150     | 911    | 1.039          | 80111  | 9.54       |
| 4   | Benzene       | 3.499     | 582569 | 4.557          | 15313  | 4.44       |
| 5   | 2-Iodopropane | 3.762     | 973    | 0.970          | 45821  | 2.87       |

## Triethanolamine


Sample: 2ul/ml ethanolamine, diethanolamine triethanolamine contrast solution, water as solvent  
 WM-54, 30m×0.53mm, 3.0µm P/N: 05915-52006  
 Column temperature: 60 C (keep 2min) 30 C/min 230 C (keep 10min)  
 Inlet temperature: 250 C Detector temperature: 250 C Detector FID  
 Carrier gas flow rate: CV mode N<sub>2</sub>, 0.04MPa Injection volume: 1µl Split ratio: 50:1

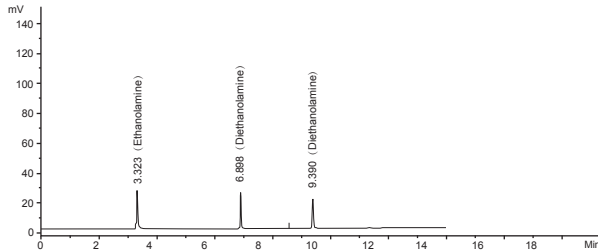

| No. | Component       | Area  | Area  | Tailing factor | Plates | Resolution |
|-----|-----------------|-------|-------|----------------|--------|------------|
| 1   | Ethanolamine    | 3.323 | 81480 | 1.2            | 38242  | 0          |
| 2   | Diethanolamine  | 6.898 | 54495 | 1.2            | 237269 | 57.5       |
| 3   | Triethanolamine | 9.390 | 61107 | 1.1            | 209097 | 36.0       |


## Epoxyethane and Dioxane in Polysorbate 80

Ethylene oxide as contrast substance 50ug/ml, water as solvent  
 WM-1, 30m×0.53mm, 1.0µm P/N: 05901-52003  
 Column temperature: 190 C Inlet temperature: 250 C Detector temperature: 280 C Detector FID  
 Carrier gas flow rate: CC mode, N<sub>2</sub>, 1.5ml/min Injection volume: 1µl Split ratio: 40:1

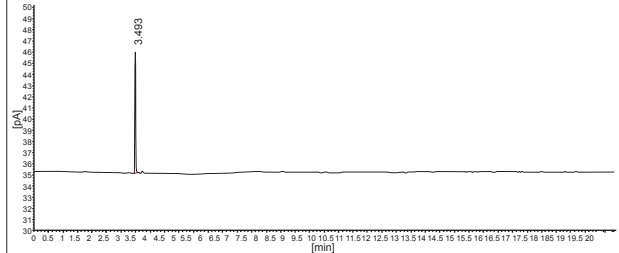


| No. | Component      | Retention | Area | Tailing factor | Plates | Resolution |
|-----|----------------|-----------|------|----------------|--------|------------|
| 1   | Ethylene oxide | 3.493     | 18.6 | 1.025          | 99784  |            |

## System Suitability

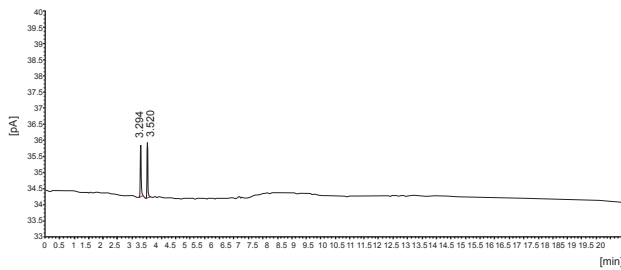


| No. | Component      | Retention | Area | Tailing factor | Plates | Resolution |
|-----|----------------|-----------|------|----------------|--------|------------|
| 1   | Acetaldehyde   | 3.294     | 2.8  | 1.395          | 97748  |            |
| 2   | Ethylene oxide | 3.520     | 3.2  | 1.297          | 97930  | 5.197      |

## Dioxane 100ug/ml, water as solvent

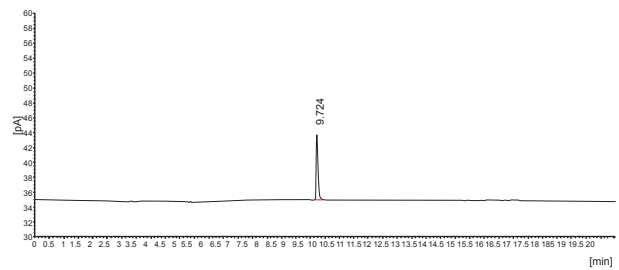


| No. | Component | Retention | Area | Tailing factor | Plates | Resolution |
|-----|-----------|-----------|------|----------------|--------|------------|
| 1   | Dioxane   | 9.724     | 38.4 | 1.400          | 121054 |            |

## Gelatin Hollow Capsules Containing Chloroethanol

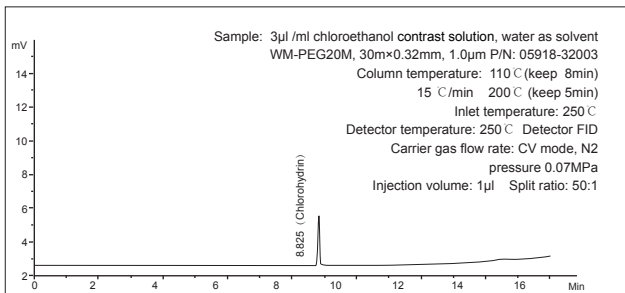

| No. | Component    | Rt    | Area  | Tailing factor | Plates | Resolution |
|-----|--------------|-------|-------|----------------|--------|------------|
| 1   | Chlorohydrin | 8.825 | 10674 | 1.0            | 134364 |            |

## Gelatin Hollow capsules containing Ethylene oxide


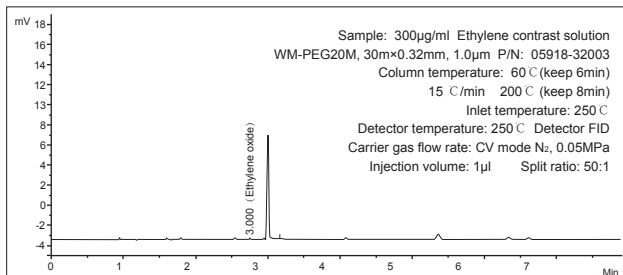


| No. | Component      | Rt    | Area  | Tailing factor | Plates | Resolution |
|-----|----------------|-------|-------|----------------|--------|------------|
| 1   | Ethylene oxide | 3.000 | 15185 | 1.0            | 91580  |            |


## Analysis of Blood Alcohol by Capillary Column

**Characteristics:** according to the GA/T 842 blood alcohol test method, the capillary column detection of blood alcohol content can also be suitable for the analysis of large amounts of water trace alcohol components.


## Analysis of Methylsilane and Propylsilane in Ethylsilane

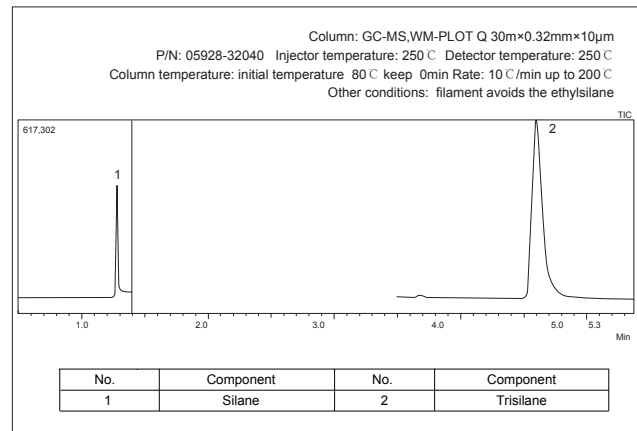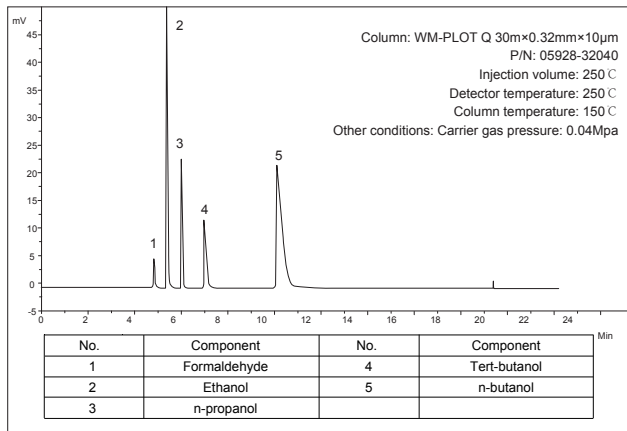

## Analysis of Alcohol Compounds

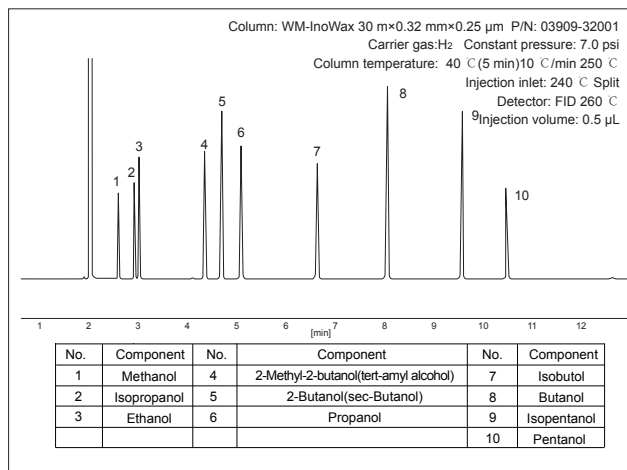


## Aromatic Volatile Organic Compounds (EPA Method 507)

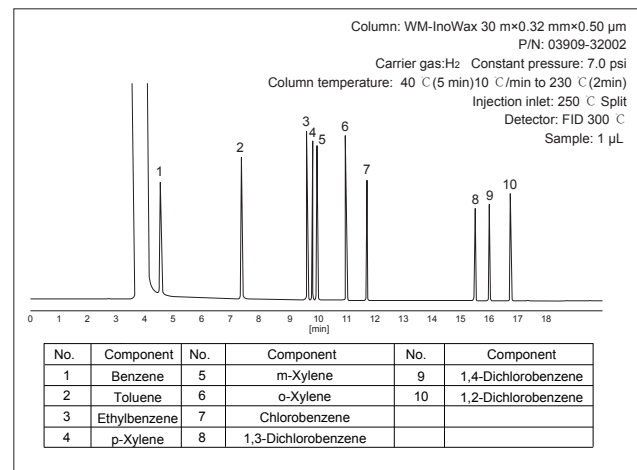


## BHA (carcinogen, butylhydroxyanisole) and BHT (dibutyl hydroxytoluene)


**Characteristics:** these two compounds have strong antioxidant ability and are often used as preservatives in food

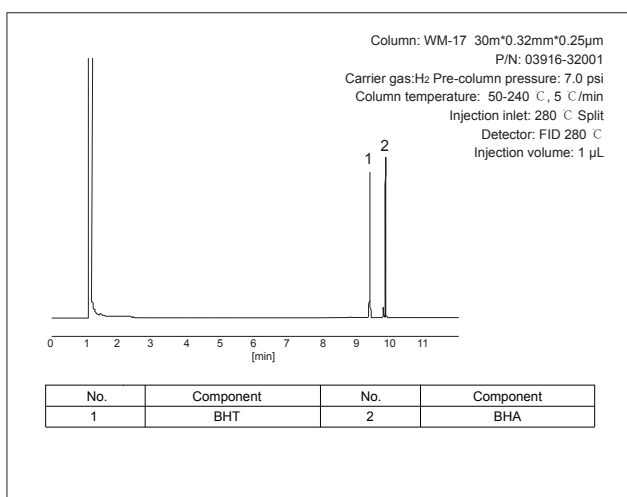

## C1-C5 hydrocarbons (analysis of hydrocarbons)

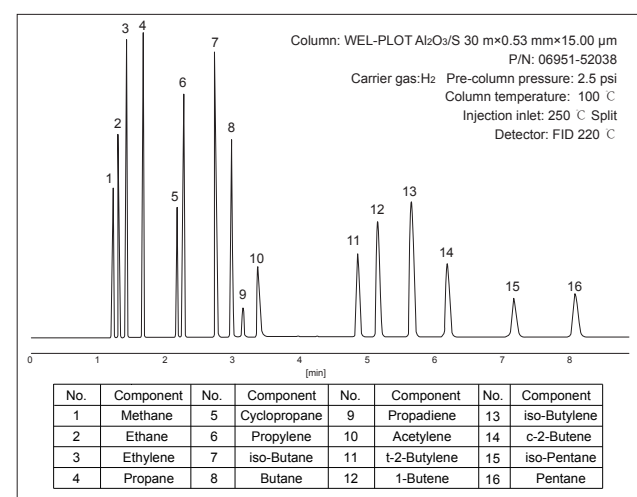


## C5-C40 Hydrocarbons (Analysis of Hydrocarbons)

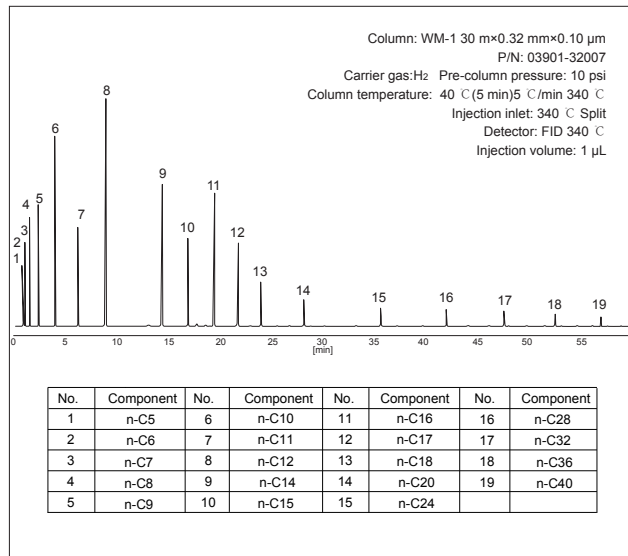


## Analysis of Ester Compounds

(Dimethyl phthalate, diethyl phthalate, phthalate esters)


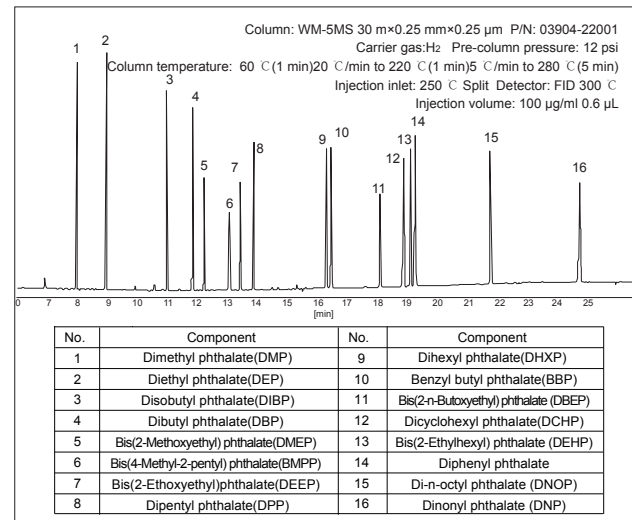


## Naphthas Analysis

(Petroleum products, chemical light oil hydrocarbon compounds)

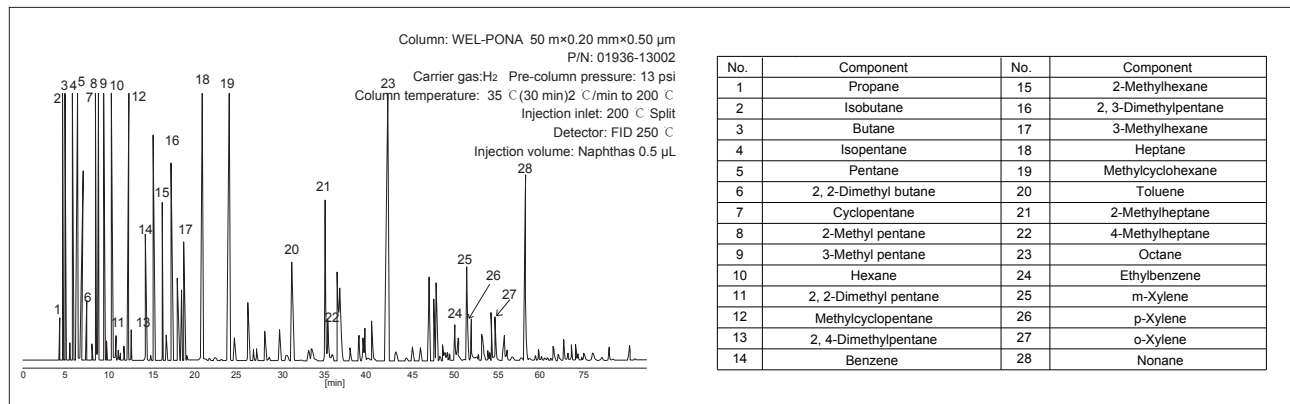


## Organics Acids Determination of Small Molecular Organic Acids PAHS Determination of Polycyclic Aromatic Hydrocarbons

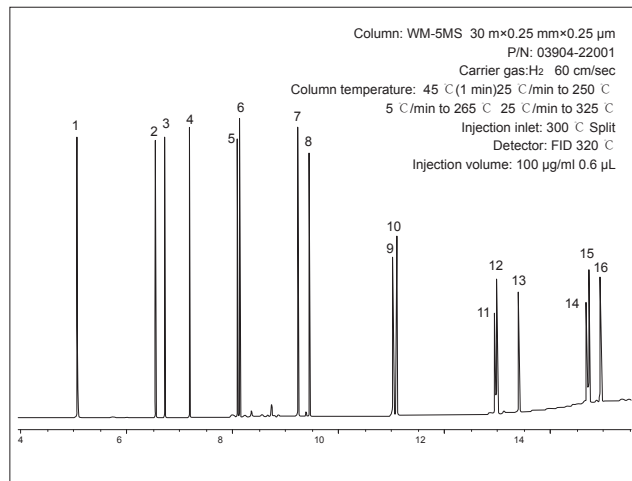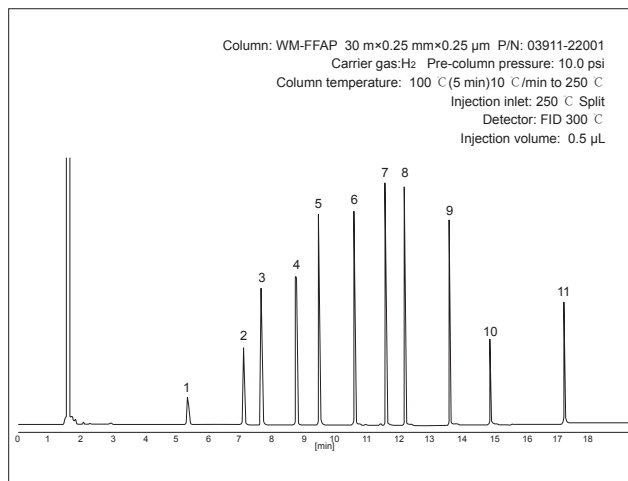

|     |                 |     |                 |     |                 |     |               |
|-----|-----------------|-----|-----------------|-----|-----------------|-----|---------------|
| No. | Component       | No. | Component       | No. | Component       | No. | Component     |
| 1   | Acetic acid     | 4   | Butyric acid    | 7   | Isocaproic acid | 10  | Octanoic acid |
| 2   | Propionic acid  | 5   | Isovaleric acid | 8   | Caproic acid    | 11  | Decanoic acid |
| 3   | Isobutyric acid | 6   | Valeric acid    | 9   | Heptanoic acid  |     |               |


|     |                |     |                          |
|-----|----------------|-----|--------------------------|
| No. | Component      | No. | Component                |
| 1   | Naphthalene    | 9   | Benz(a)anthracene        |
| 2   | Acenaphthylene | 10  | Chrysene                 |
| 3   | Acenaphthene   | 11  | Benzo(b)fluoranthene     |
| 4   | Fluorene       | 12  | Benzo(k)fluoranthene     |
| 5   | Phenanthrene   | 13  | Benzo(a)pyrene           |
| 6   | Anthracene     | 14  | Indeno(1, 2, 3-cd)pyrene |
| 7   | Fluoranthene   | 15  | Dibenz(a, h)anthracene   |
| 8   | Pyrene         | 16  | Benzo(g, h, i)perylene   |

## Determination of Refinery Gas

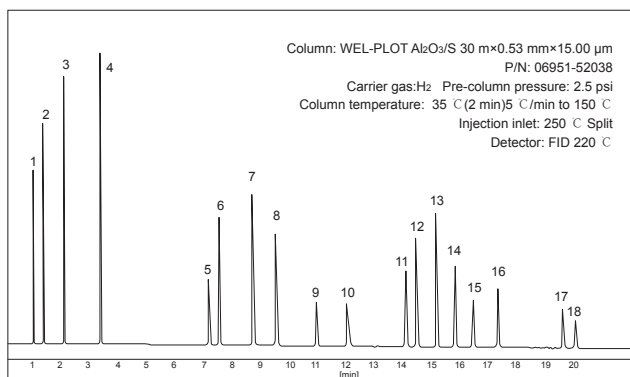


|     |              |     |            |     |              |     |               |
|-----|--------------|-----|------------|-----|--------------|-----|---------------|
| No. | Component    | No. | Component  | No. | Component    | No. | Component     |
| 1   | Methane      | 6   | Propylene  | 11  | t-2-Butylene | 16  | Pentane       |
| 2   | Ethane       | 7   | iso-Butane | 12  | 1-Butene     | 17  | 1,3-Butadiene |
| 3   | Ethylene     | 8   | Butane     | 13  | iso-Butylene | 18  | Propyne       |
| 4   | Propane      | 9   | Propadiene | 14  | c-2-Butene   |     |               |
| 5   | Cyclopropane | 10  | Acetylene  | 15  | iso-Pentane  |     |               |

## Solvent I Determination of Residual Solvent

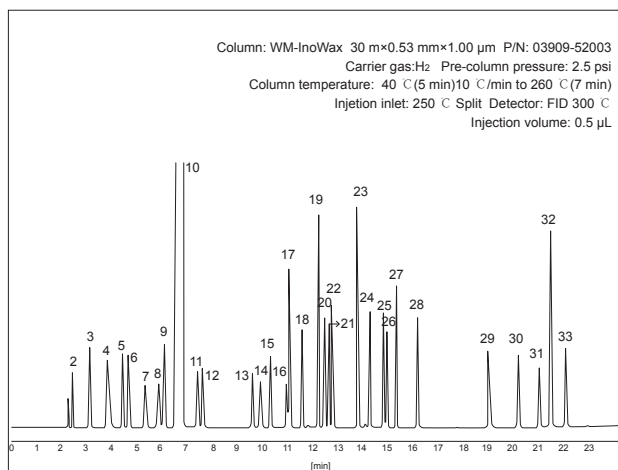


|     |                      |     |                        |
|-----|----------------------|-----|------------------------|
| No. | Component            | No. | Component              |
| 1   | Pentane              | 18  | iso-Butanol            |
| 2   | Hexane               | 19  | iso-Amyl acetate       |
| 3   | Cyclohexane          | 20  | Ethylbenzene           |
| 4   | Triethylamine        | 21  | p-Xylene               |
| 5   | Acetone              | 22  | m-Xylene               |
| 6   | Methyl acetate       | 23  | o-Xylene               |
| 7   | Tetrahydrofuran(THF) | 24  | Propylbenzene          |
| 8   | Tetrachloromethane   | 25  | tert-Butylbenzene      |
| 9   | Ethyl acetate        | 26  | Pentanol               |
| 10  | Methanol             | 27  | Phenylethylene         |
| 11  | Methylene chloride   | 28  | Cyclohexanone          |
| 12  | Ethanol              | 29  | Acetic acid            |
| 13  | Acetonitrile         | 30  | Benzaldehyde           |
| 14  | Chloroform           | 31  | DMSO(methyl sulfoxide) |
| 15  | Toluene              | 32  | Ethylene glycol        |
| 16  | 1,4-Dioxane          | 33  | Acetophenone           |
| 17  | Butyl acetate        |     |                        |

## Solvent II Analysis and Determination of Residual Solvent

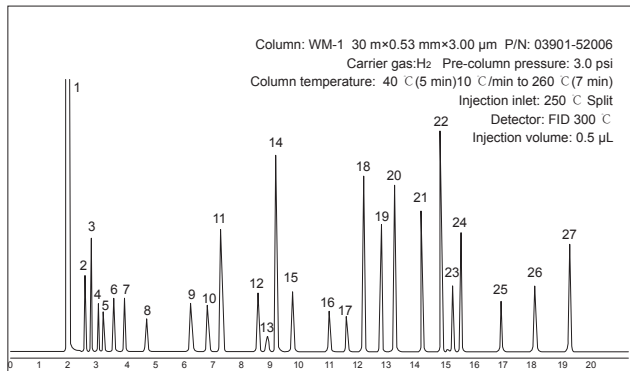

|     |                      |     |                               |
|-----|----------------------|-----|-------------------------------|
| No. | Component            | No. | Component                     |
| 1   | Methanol             | 15  | Triethylamine                 |
| 2   | Ethanol              | 16  | Pyridine                      |
| 3   | Acetonitrile         | 17  | N,N-dimethylformamide         |
| 4   | Acetone              | 18  | Toluene                       |
| 5   | Isopropanol          | 19  | Dimethyl sulfoxide (DMSO)     |
| 6   | Pentane              | 20  | Butyl acetate                 |
| 7   | Methylene chloride   | 21  | N, N-dimethylacetamide (DMAC) |
| 8   | Propanol             | 22  | Ethylbenzene                  |
| 9   | sec-Butanol          | 23  | Cyclohexanone                 |
| 10  | Chloroform           | 24  | Phenylethylene                |
| 11  | Tetrahydrofuran(THF) | 25  | Benzaldehyde                  |
| 12  | Butanol              | 26  | tert-Butylbenzene             |
| 13  | Tetrachloromethane   | 27  | Acetophenone                  |
| 14  | Ethylene glycol      |     |                               |

## Determination of Substituted Aniline Compounds

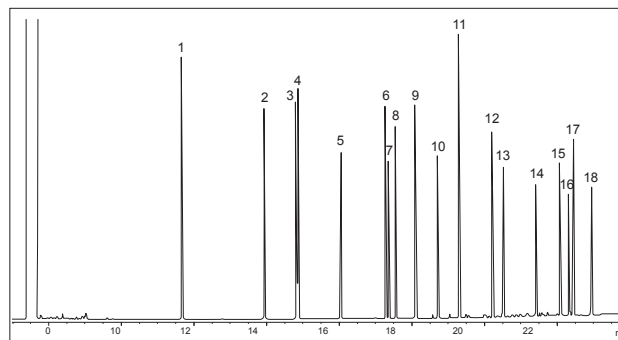




| No. | Component       | No. | Component               | No. | Component                       |
|-----|-----------------|-----|-------------------------|-----|---------------------------------|
| 1   | Aniline         | 7   | 2,4,6-Trichloroaniline  | 13  | 2,6-Dichloro-4-nitroaniline     |
| 2   | 2-Chloroaniline | 8   | 3,4-Dichloroaniline     | 14  | 2-Bromo-6-chloro-4-nitroaniline |
| 3   | 3-Chloroaniline | 9   | 3-Nitroaniline          | 15  | 2-Chloro-4,6-dinitroaniline     |
| 4   | 4-Chloroaniline | 10  | 2,4,5-Trichloroaniline  | 16  | 2,6-Dibromo-4-nitroaniline      |
| 5   | 4-Bromoaniline  | 11  | 4-Nitroaniline          | 17  | 2,4-Dinitroaniline              |
| 6   | 2-Nitroaniline  | 12  | 2-Chloro-4-nitroaniline | 18  | 2-Bromo-4,6-dinitroaniline      |




Column: WM-5ms 30 m×0.25 mm×0.50 μm  
P/N: 03904-22002  
Carrier gas: H<sub>2</sub> 33 cm/sec Measured at 150 °C  
Column temperature: 40 °C (5 min) 12 °C/min to 300 °C (10 min)  
Injection inlet: 250 °C split  
Detector: FID 325 °C  
Injection volume: 0.5 μL

## Gas Phase Accessories

### 3.1 Gas Generator

Product description: gas generator is safe, reliable and easy to operate, if turn on the power, it can produce high purity carrier gas with stable pressure, which is suitable for various GC manufacturers as an ideal substitute for gas cylinder.

| Product                        | Type     | Figure                                                                              |
|--------------------------------|----------|-------------------------------------------------------------------------------------|
| High-purity hydrogen generator | GH-300   |    |
| High-purity hydrogen generator | GH-500   |                                                                                     |
| High-purity hydrogen generator | GH-400   |                                                                                     |
| High-purity hydrogen generator | GH-600   |                                                                                     |
| High-purity hydrogen generator | GN-300   |   |
| High-purity hydrogen generator | GN-500   |                                                                                     |
| Low noise air pump             | GA-2000A |  |
| Low noise air pump             | GA-5000A |                                                                                     |
| Low noise air pump             | GA-3000  |                                                                                     |

| Product                         | Type    | Figure                                                                                |
|---------------------------------|---------|---------------------------------------------------------------------------------------|
| Nitrogen hydrogen air generator | NA-300A |    |
| Nitrogen hydrogen air generator | NA-500A |                                                                                       |
| Nitrogen hydrogen air generator | HA-300A |   |
| Nitrogen hydrogen air generator | HA-500A |                                                                                       |
| Nitrogen hydrogen air generator | GX-300A |  |
| Nitrogen hydrogen air generator | GX-500A |                                                                                       |




### 3.2 Gas Phase Accessories

Product description: with reliable quality, can match all kinds of gas chromatographs (Agilent, Shimazu, Platinum Elmer, Syme Technology, Brook, etc.) perfectly.

#### 3.2.1 Injection Septa

Septum pollution or loss under high temperature, will lead to ghost peaks; Septa leakage, will lead to increased retention time and detector signal noise, decreased head pressure. It is recommended that the injection septa need to be changed frequently during daily use of the gas chromatograph.

**Tab 3.1 Common fault of injection septa and solutions**

| Phenomenon                                                                                                             | Possible Reasons                                                                                                                 | Solutions                                                                                                                                                         |
|------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Extra peak/<br>round peak<br>       | Septa loss                                                                                                                       | If the extra peak disappears after closing the injector heater, it is suggested to change to high temperature septa or reduce the inlet temperature for analysis. |
| Post-peak baseline<br>variation<br> | Severe leakage at the septa during the short time after injection, which is usually caused by a larger diameter injection needle | Change septa and use a smaller diameter injection needle                                                                                                          |
| Post-peak baseline<br>variation<br> | Carrier gas leakage occurs at the injector septa or column junction                                                              | Check for leaks, if any, replace the septa, or tighten the column junction                                                                                        |



### Suggestions for the Maintenance of Injection Septa:

- The use temperature of the spacer shall not exceed the recommended temperature
- Check and replace regularly
- Use an autosampler and the septa sweeping function if possible

**Tab 3.2 Classification of injector septa**

| Type                                         | Leachability | Lifetime | Temperature Limit |
|----------------------------------------------|--------------|----------|-------------------|
| BTO® (Drain and temperature optimized septa) | √√√          | √        | up to 400 °C      |
| Advanced Green 3™ (Premium green septa)      | √√           | √√       | up to 350 °C      |
| Marathon™ (Long lifetime septa)              | √            | √√√      | up to 350 °C      |

(√√√ = best    √√ = better    √ = good)

### Drain and temperature optimized septa (BTO®)



- Extended temperature range, lowest loss
- Max. temp. is 400 C
- Each batch of septa is tested for loss by GC-FID
- Plasma treatment can eliminate adhesion and contamination at the injector
- Pre-aging, ready to use
- Packed in a clean glass bottle, clean and convenient

### Long lifetime septa (Marathon™)



- The best septa for automatic injector with great operation
- Max. temp. 350 C
- Preperforation can avoid clastic formation and prolong life
- Each septa can tolerate up to 400 injections
- Plasma treatment can eliminate the adhesion at the injector inlet
- Packed in a clean glass bottle, clean and convenient


### Premium green septa (AG3™)




- Real long lifetime, high temperature resistant green septa
- High service temperature 350 C
- Each septa is subjected to more injections
- As high-performance alternative of green septa
- Best for low-loss, MS capillary column

### Comparison septa leachability

- A) BTO septa
- B) AG3 septa
- C) Competing manufacturer's high temperature red spacer
- D) Competitor's low loss green septa



**Fig 3.1 Comparison septa leachability**

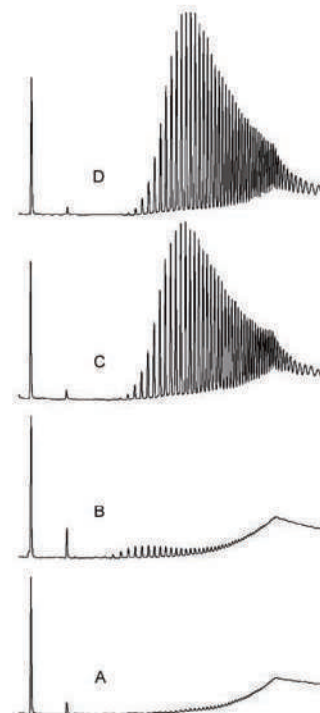




### 3.2.2 Graphite Ferrule






Improper use of sealing ferrule results in inconsistent chromatographic peaks and unreliable analytical results. Specifically, improper sealing ferrule can cause air and other contaminants and into the instrument system, seriously affecting column efficiency and detector performance. For optimal performance, replace the sealing ferrule every time the column is replaced or maintained.

- To minimize problems, install the sealing ferrule with the following precautions:
- Don't screw too tight-tighten the column nut with your fingers and then tighten it with a wrench
- Prevent pollution and keep clean
- Before reusing, check the seal gasket for cracks, debris, or other damage with a magnifying glass. Replace the seal gasket when installing a new column or injector/detector component

#### Guide to sealing ferrule selection

| Type                                                                                                   | Temperature limit | Usage                                                                                                                                                                                           | Advantage                                                                                                                                        | Limitaion                                                                                                                                                                                                  |
|--------------------------------------------------------------------------------------------------------|-------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>Carbon (100%)</p>  | 450 °C            | <ul style="list-style-type: none"> <li>• Capillary column general</li> <li>• Suitable for FID and NPD</li> <li>• Recommended for high temperature and cold columns</li> </ul>                   | <ul style="list-style-type: none"> <li>• Easy to use, stable seal</li> <li>• Higher temperature upper limit</li> <li>• Easy to remove</li> </ul> | <ul style="list-style-type: none"> <li>• It is not recommended for MS and oxygen sensitive detectors</li> <li>• Soft, easy to deformation or damage</li> </ul>                                             |
| <p>Vespe/Carbon</p>  | 400 °C            | <ul style="list-style-type: none"> <li>• Capillary column</li> <li>• It is recommended for MS and oxygen sensitive detectors</li> <li>• The most reliable leak-free connection</li> </ul>       | <ul style="list-style-type: none"> <li>• Mechanical stability</li> <li>• Long life</li> </ul>                                                    | <ul style="list-style-type: none"> <li>• Cannot be reused</li> <li>• It flows at high temperatures</li> <li>• It must be retightened</li> </ul>                                                            |
| <p>100% Vespe</p>   | 350 °C            | <ul style="list-style-type: none"> <li>• Constant temp operation</li> <li>• Reusable and easy to remove</li> <li>• It is an excellent sealing material for connecting metal or glass</li> </ul> | <ul style="list-style-type: none"> <li>• Stable mechanical properties</li> <li>• Long lifetime</li> <li>• Reusable and easy to remove</li> </ul> | <ul style="list-style-type: none"> <li>• The program may leak after heating up several times</li> <li>• It's going to run off at high temperatures</li> <li>• It must be retightened frequently</li> </ul> |

### 3.2.3 Ordering Information of GC Accessories

| P/N         | Product               | Specification                                                                                                         | Pack  | Picture                                                                               |
|-------------|-----------------------|-----------------------------------------------------------------------------------------------------------------------|-------|---------------------------------------------------------------------------------------|
| 00832-00001 | Silanized glass wool  | Welchrom® max temp. 400 °C, 0.5g/pcs, 1bag                                                                            | 1 bag |  |
| 00832-00004 | Two-way valve         | Welchrom® no variable diameter, 3mm outer diameter (Stainless steel) : Suitable for 2mm inner diameter column tube, 1 | 1pk   |  |
| 00832-00005 | Three-way valve       | Welchrom® no variable diameter, 3mm outer diameter (Stainless steel) : Suitable for 2mm inner diameter column tube, 1 | 1pk   |                                                                                       |
| 00832-00006 | Nut                   | Welchrom® 3mm outer diameter (Stainless steel) suitable for 2mm inner diameter column tube, 1                         | 1pk   |  |
| 00832-00007 | Gas path on/off valve | Welchrom® 3mm outer diameter                                                                                          | 1     |  |
| 00832-00008 | Graphite ferrule      | Max 400 °C, Welchrom® Suitable for column inner diameter: 3mm, 1                                                      | 1     |  |
| 00832-00013 | Graphite ferrule      | Max 400 °C, Welchrom® Suitable for column inner diameter: 2mm, 1                                                      | 1     |                                                                                       |

| P/N         | Product               | Specification                                                                         | Package | Picture                                                                             |
|-------------|-----------------------|---------------------------------------------------------------------------------------|---------|-------------------------------------------------------------------------------------|
| 00832-00014 | Graphite ferrule      | Max temp. 400 °C, Welchrom® suitable column inner diameter 0.53mm                     | 1       |  |
| 00832-00015 | Graphite ferrule      | Max temp. 400 °C, Welchrom® suitable column inner diameter 0.32mm                     | 1       |                                                                                     |
| 00832-00009 | Soap bubble flowmeter | Welchchrom® contains a glass flowmeter, a 50cm hose, a rubber head, 100ml (glass)     | 1 pcs   |  |
| 00832-00010 | Gas pipeline          | Welchchrom® outer diameter 3mm, inner diameter 2mm, materials: teflon tube            | 1 meter |  |
| 00832-00011 | Deoxidation tube      | Welchchrom® color changing type, organic glass material                               | 1 pcs   |  |
| 00832-0001  | Gas path purifier     | Welchchrom® packing materials: allochroic silicagel activated carbon, molecular sieve | 1       |  |

## Method A: Determination of organochlorine pesticide residues - Chromatography

### Determination of 9 organochlorine pesticide residues

#### 1. Method introduction

The homogenized samples will be separated by adding sodium chloride and dichloromethane after extraction with water and acetone. Concentrate organic phase, then redissolve with petroleum ether and sulfonate with concentrated sulfuric acid. Through decompression and concentration and redissolve with petroleum ether for GC-ECD analysis and determination.

#### 2. Sample preparation

1

After precise weighing and homogenizing, put 2g samples into 100ml conical flask and soaked in 20ml water overnight.

2

Add acetone 40ml precisely, ultrasound for 30 mins (using acetone to make up the reduced weight);

3

Add 6g NaCl, 30ml dichloromethane, ultrasound for 15 mins (using acetone to make up the reduced weight);

4

Transfer organic phase to a 100ml conical flask containing an appropriate amount of anhydrous sodium sulfate and placed for 4 hours.

5

Weigh 35ml precisely and through decompression and concentration under 40 °C to nearly dry, then add a small amount of petroleum ether (60-90 °C) to converse several times.

6

Dissolve the petroleum ether and transfer petroleum ether to 10ml centrifuge tube with plug. Dilute the petroleum ether (60-90 °C) to 5ml.

7

Carefully add 1ml sulfuric acid, shake for 1 minute.

8

Centrifuge at 3000rpm for 10 minutes. Take 2ml of the supernatant for precision measurement and place it in a graduated concentrator.



9

Through decompression and concentration under 40 °C to nearly dry, add petroleum ether (60-90 °C) to a constant volume of 1mL for GC-ECD analysis.

### 3. GC Chromatographic condition

GC Chromatographic condition  
 Column: WM-1701 (30m×0.32mm×0.25μm),  
 Column temperature: 100 C (0min) 10 C/min→220 C (0min) 8 C/min →250 C (10min)  
 Carrier gas: N<sub>2</sub>  
 Injector: 250 C, splitless injection  
 Detector: ECD 300 C  
 Peak: 1- α- benzene hexachloride, 2-γ-benzene hexachloride, 3-β- benzene hexachloride, 4-δ- benzene hexachloride, 5-ε- benzene hexachloride, 6- p,p'-DDE, 7- o,p'-DDT, 8- p,p'-DDD, 9- p,p'-DDT

GC-ECD Chromatogram of 9 organochlorine standard solutions

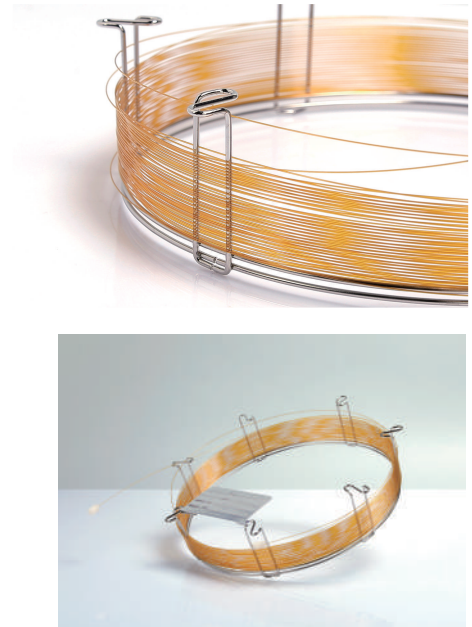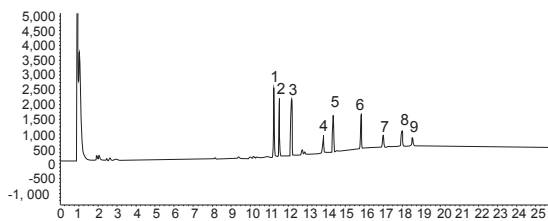

### 4. Related Products

The homogenized samples will be separated by adding sodium chloride and dichloromethane after extraction with water and acetone. Concentrate organic phase, then redissolve with petroleum ether and sulfonate with concentrated sulfuric acid. Through decompression and concentration and redissolve with petroleum ether for GC-ECD analysis and determination.

| P/N         | Product    | Specification             |
|-------------|------------|---------------------------|
| 03907-32001 | WM-1701    | WM-1701 30m×0.32mm×0.25μm |
| 03902-32001 | WM-5 GC Ca | WM-5 30m×0.32mm×0.25μm    |

Variety of specifications, welcome to consult

## Determination of 22 Organochlorine Pesticide Residues

### 1. Method introduction

After the homogenized samples are extracted by water and acetonitrile, the two phases can be stratified by salting out pack. The acetonitrile phase was concentrated and then redissolve with cyclohexane-ethyl acetate (1:1) solution, purified by gel chromatography and florel silica column. Through decompression and concentration and redissolve with petroleum ether for GC-ECD analysis and determination. analysis and determination.

### 2. Sample preparation

1

After precisely weigh and homogeneity, put 1.5g samples in a 50mL centrifuge tube and soak it in 10ml water for 2 hours.

2

Precisely add 15ml acetonitrile and extract by violent shock for 1 min.

3

Add QuEChERS salting out packs (4g anhydrous magnesium sulfate +1g sodium chloride) and shake violently for 1 min.

4

After centrifugation at 4000rpm for 1 min precisely transfer 10mL acetonitrile phase and through decompression and concentration at 40 C.

5

Transfer 10mL solution of ethyl acetate - cyclohexane (1:1) to a 10mL measuring flask by several times, and keep volume at 10ml.

6

Take 5 ml of supernatant to be purified by GC. Column used is Welch Bio-Beads S-X3 400×25mm.

7

Collect purification liquid for 18-30min, concentrate at 40 °C under decompression to nearly dry, and then add 1ml n-hexane for resolution. Collect eluent according to the detector to check the peak of organochlorine.

8

Use Florisil silica column for purification (Florisil PR 1000mg/6ml).

9


After purification, the samples can be concentrated to near dry with a nitrogen blower, and add 1ml isooctane vortex for GC-ECD analysis.

Note: The boiling range of petroleum ether used in this experiment is 60-90 °C

### 3. Chromatographic analysis


Column: Welch Bio-Beads S-X3 400×25mm  
Flow rate: 5ml/min  
Mobile phase: cyclohexane/ethyl acetate=1:1  
Column temperature: room temperature(about 24 °C)

(1) Chromatogram of 22 kinds of organochlorine standard solutions GPC

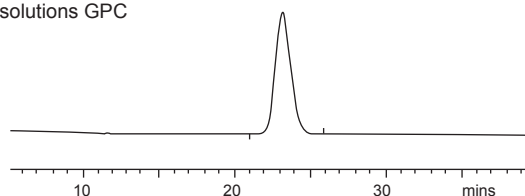

GC chromatographic condition  
Column: WM-17 (30m×0.25mm×0.25µm),  
Column temperature: 70 °C(1min)10 °C/min→180 °C(5 min)5 °C/min →220 °C(0 min)100 °C/min→280 °C(8 min)  
Carrier gas: N<sub>2</sub>, 1.3ml/min  
Injector: 240 °C, splitless injection  
Detector: ECD 300 °C  
Chromatographic : 1-Hexachlorobenzene, 2-α-Benzene hexachloride, 3-Quintozene, 4-γ-benzene hexachloride, 5-β-benzene hexachloride, 6-Heptachlor, 7-δ-benzene hexachloride, 8-Aldrin, 9-Oxychlordan e Isomer, 10-Ethylcarboxamido Adenosine, 11-Heptachlor-endo-epoxide, 12-Trans-chlordane, 13-Cis-chlordane, 14-α-endosulfan, 15- p, p'-DDE, 16-Dieldrin, 17-Endrin, 18-o, p'-DDT, 19- p, p'-DDD, 20-β-endosulfan, 21- p, p'-DDT, 22- Sulfate

(2) Chromatogram of 22 kinds of organochlorine standard solutions GC-ECD

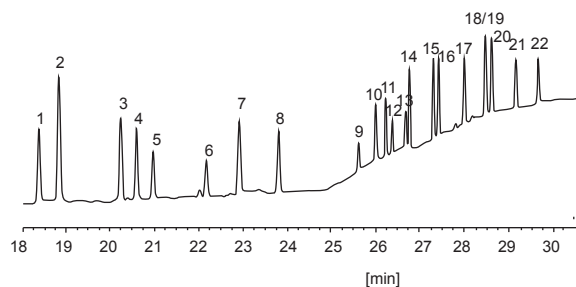

### 4. Related products

| P/N         | Product                                | Specification                                                                                                              |
|-------------|----------------------------------------|----------------------------------------------------------------------------------------------------------------------------|
| 03916-32001 | WM-17 GC Capillary Column(HPLC column) | WM-17 30m×0.25mm×0.25µm                                                                                                    |
| 01901-22001 | WEL-1 GC (Verification column)         | WEL-1 30m×0.25mm×0.25µm                                                                                                    |
| 00530-20000 | QuEChERS Extraction Bag                | QuEChERS extraction bag, initial method (without buffer salt) 4g magnesium sulphate, 1g NaCl, use in10g samples, 50pcs/box |
| 00516-20007 | Welchrom® SPE Column                   | Welchrom® Florisil PR,1g/6ml, 30pk                                                                                         |
| 00823-00002 | GPC Column                             | Welch Bio-Beads S-X3, 200-400 mesh,                                                                                        |


Variety of specifications, welcome to consult

## Method B: Determination of organochlorine pesticide residues - Chromatographic method

### 1. Method introduction

After the homogenized samples are extracted by water and acetonitrile, purified by gel chromatography and florel silica column. Through decompression and concentration, redissolve with petroleum ether for GC- NPD/FPD analysis and determination.

### 2. Sample preparation

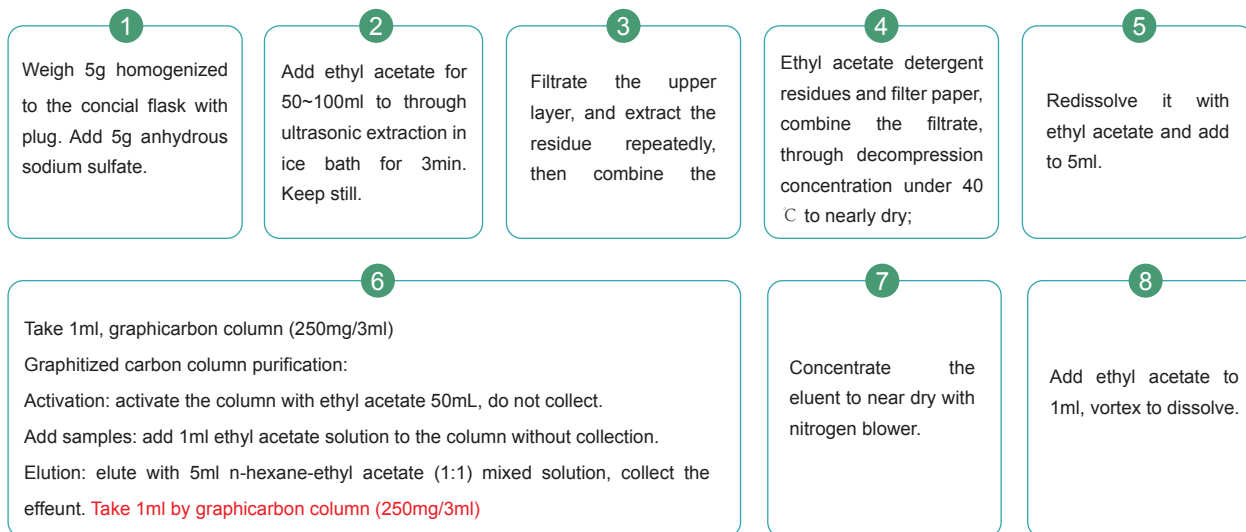

### 3. Related products

| P/N         | Product                   | Specification                                                      |
|-------------|---------------------------|--------------------------------------------------------------------|
| 03916-22001 | WM-17 GC capillary column | WM-17 30m×0.25mm×0.25μm                                            |
| 03902-22001 | WM-5 GC capillary column  | WM-5 30m×0.25mm×0.25μm                                             |
| 00551-20000 | QuEChERS extraction bag   | QuEChERS extraction bag, 5.0g anhydrous sodium sulfate, 50 pcs/box |
| 00517-20012 | Welchrom® SPE column      | Welchrom® Carb, 250mg/3ml, 50pk                                    |


Variety of specifications, welcome to consult

## Method C: Determination of pyrethroid pesticide residues - Chromatographic method

### 1. Method introduction

After the homogenized samples were extracted by ultrasound with mixed solution of petroleum and ether-acetone, dehydrate with anhydrous sodium sulfate and purify by special column for pyrethroid. Concentrate and redissolve, and add petroleum ether to have a constant volume for GC-ECD analysis.

### 2. Sample preparation

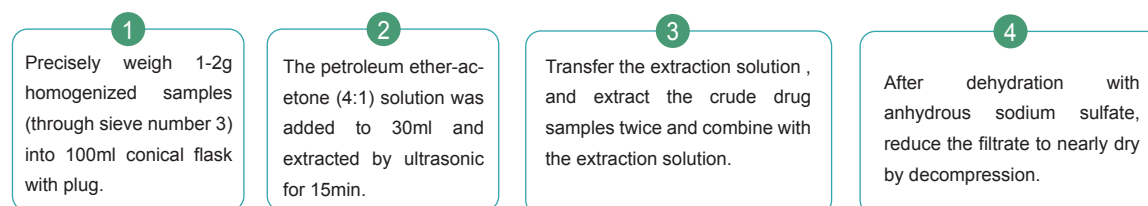

5

Used a small amount of petroleum ether repeatedly until acetone was removed and then dissolve with 5ml petroleum ether.

Purify with special column for pyrethroid:

Activation: Activate column by petroleum ether-ethyl ether (4:1) mixed solution of 20mL, without collection.

Sample loading: add 5ml petroleum ether solution to the column and collect the outflow.

Elution: elute with 90ml mixed solution of petroleum and ether-ethyl ether (4:1) and collect the elution.

Reduce pressure and concentrate the sample effluent and eluent under 40 C to nearly dry.

Repeat the operation with 4ml of petroleum ether until the ethyl ether is removed, dissolve with a small amount of petroleum ether and transfer it to a 5ml measuring bottle, make a constant volume with petroleum ether, shake well.

Note: The boiling range of petroleum ether used in this experiment is 60-90 C


### 3. Analysis of Chromatogram

Column: WM-5 30m×0.32mm×0.25μm

Detector: ECD

Inlet temperature: 270 C, detector temperature 330 C, splitless injection

Temperature program: 160 C (1min)10 C/min→278 C (0.5min), 1 C/min →290 C (5min)

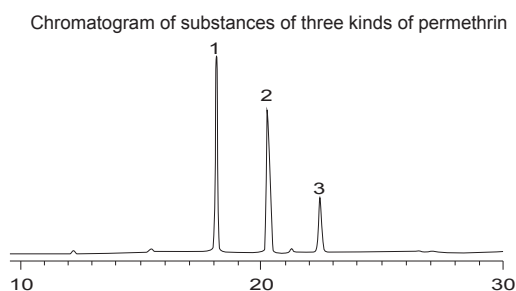

### 4. Related products

| P/N         | Products                 | Specification          |
|-------------|--------------------------|------------------------|
| 03902-32001 | WM-5 GC capillary column | WM-5 30m×0.32mm×0.25μm |

Variety of specifications, welcome to consult

## Method D: Determination of pyrethroid pesticide residues-MS

### 1. Method introduction

Extract homogenized samples which were soaked in 1% aqueous acetic acid solution with acetonitrile. Then stratify by salting out bag. After centrifugation, take the supernatant to be purified with QuEChERS purification tube. Concentrate to have a constant volume for GC /MS or LC/MS analysis.

### 2. Sample preparation

1

Precisely weigh tested product 3g to 50mL polystyrene centrifuge tube with plug

2

Add 15ml 1% glacial acetic acid solution and soak in vortex for 30min.

3

Precisely add 15ml acetonitrile and 100 μl internal standard solution;

4

Extract with violent oscillation for 5 minutes.



5

Add QuEChERS salting out bag and shake violently for 3min, then cool in the ice bath for 10 min.

6

After centrifugation at 4000rpm for 5min, take 9ml supernatant and added the QuEChERS purification tube for 5min of violent oscillation.

7

After centrifugation at 4000rpm for 5min, take 5 ml supernatant and concentrate at 5ml 40 C to about 0.4mL, and stabilize with acetonitrile to 1mL.

8

Mix the vortex with a 0.22μm nylon filter for instrumental analysis.



### 3. Related products

| P/N         | Products                                        | Specification                                                                                                      |
|-------------|-------------------------------------------------|--------------------------------------------------------------------------------------------------------------------|
| 03904-22001 | WM-5MS GC Capillary Column (1.GC-MS/MS)         | WM-5MS 30m×0.25mm×0.25µm                                                                                           |
| 960-04023   | Boltimate® C18 (Core-Shell) Column (2.LC-MS/MS) | Boltimate® C18, 2.7µm, 90Å, 3.0×150mm                                                                              |
| 00528-20000 | QuEChERS extraction bag                         | QuEChERS extraction bag, AOAC method, 6g magnesium sulfate, 1.5g sodium acetate, 50 pcs/box                        |
| 00581-20021 | QuEChERS extraction tube                        | QuEChERS extraction tube-15ml, 900mg MgSO <sub>4</sub> , 300mg PSA, 300mg C18E, 300mg Silica, 90mg GCB, 50 pcs/box |

## Method E: Determination of pesticide residue-MS method

### Sample preparation

#### 1. Extration steps

Weigh 5g samples and add 1g sodium chloride, then shake. Continue to add 50mL acetonitrile, homogenized, centrifuge for 5min (4000r/min), and remove supernatant. Add 50mL acetonitrile into the precipitation, homogenized, centrifuge for 5min (4000r/min), then transfer the supernatant and combine. Concentrate the supernatant in a water bath at 40 °C to 3-5mL, then dilute and redissolve with acetonitrile to 10mL, shake well, and set aside. Weigh 5g samples, and add 1g NaCl.

#### 2.Celanup steps

##### Method 1:

Welchrom® QuEChERS specification: anhydrous magnesium sulfate 1200mg, N-propyl ethylenediamine (PSA) 300mg, and measure C18E 100mg and 3mL of the test product solution prepared by direct extraction method in a centrifuge tube, which was fully mixed by vortex, centrifuge for 5min (4000r/min), and transfer the supernatant.

##### Method 2:

SPE column: Welchrom®BRP, specificaiton: 200mg/6mL

Sample loading: The test sample solution is 3mL, purify with the column, collect all the purification liquid, mix.

##### Method 3:

SPE column: Welchrom® Carb/NH<sub>2</sub>, specification: 250mg/250mg/6mL

Actviation: 10mL acetonitrile-toluene(3:1), discard.

Sample loading: collect 2mL of the test sample solution prepared by the direct extraction method and collect in a heart-shaped flask.

Elution: 20mL acetonitrile-toluene (3:1) elute, press and collect in a heart-shaped flask.

Redissolve: cycle the collected liquid to dry in a water bath at 40 °C, then transfer with acetonitrile and dilute to 2mL.

Determination method: accurately absorb 1mL of each substrate mixed control solution and test sample solution, and accurately add 0.3ml of internal standard, mix, filter, and take the additional filtrate for detection, and calculate according to the standard curve method of internal standard.

### 3. Related products

| P/N          | Procut          | Specification                                                                                                                  |
|--------------|-----------------|--------------------------------------------------------------------------------------------------------------------------------|
| 00522-20014  | SPE column      | Welchrom® BRP,200mg/6mL,30pk                                                                                                   |
| 00527-20010  | SPE column      | Welchrom® Carb/NH <sub>2</sub> ,250mg/250mg/6mL,30pk                                                                           |
| 005PM-077-50 | QuEChERS        | QuEChERS extration-15ml, 1200mg MgSO <sub>4</sub> , 300mg PSA, 100mg C18E, 50 pcs/box                                          |
| 00837-05006  | Centrifuge tube | Welchrom® centrifuge tube, disposable centrifugal tube, flat cap, conial, RCF12000xg, bag, without sterilization, 50mL, 50/pcs |
| 00837-05002  | Centrifuge tube | Welchrom® centrifuge tube, centrifuge tube, flat cap, RCF12000xg, bag, without sterilization, 15mL, 50/pcs                     |



|             |                |                                                                                    |
|-------------|----------------|------------------------------------------------------------------------------------|
| 00824-31001 | SPE device     | Welch SPE device, 12 port                                                          |
| 00821-32291 | Caps and septa | Pre-slit white PTFE/white silicone septa, 9mm blue short screw-thread cap, 100/pk. |
| 00821-40927 | Sample vial    | Welchrom® 2mL wide opening short screw-thread vial, clear, 11.6×32mm, 100/pk       |
| 03916-22001 | GC column      | WM-17,30m×0.25mm×0.25µm                                                            |

## Technical Reference

### 5.1 Selection of GC Column

In actual work, if the separated component has enough thermal stability and volatility, GC separation mode should be considered first during analysis. Compared with LC, GC has advantages as follows: faster analysis speed, great repeatability, lower cost, and its column efficiency usually has a higher order of magnitude.

#### How to Select Correct Capillary Column

For separation problem of a kind of sample, selecting a suitable capillary column is a very important task, which concerns a series of principles.

In general, this selection principles are around three requirements as follows: sample component should have suitable retention value, the analysis speed should be fast and the analysis time should be short.


According to GC basic principles and actual requirements, we need to consider several main influencing factors, such as stationary phase, inner diameter of column, column length and film thickness.

#### 5.1.1 Selection of Stationary Phase

Stationary phase of polydimethylsiloxane has high thermal stability and it keeps liquid state from  $-60\text{ }^{\circ}\text{C}$  to  $350\text{ }^{\circ}\text{C}$ , which has wide application range among GC. When other groups, such as -CN or phenyl, replace the alkyl of siloxane, the polarity of the stationary phase will change and columns with polarity and selectivity appear.

Polyethylene glycol (PEG) is another widely used stationary phase with polarity, among which PEG 20M (WM is about 20,000) is the most popular one. The hydroxyl groups of polyethylene glycol chain react with various functional groups, which can change the selectivity and improve the thermal stability of stationary phase. FFAP, for example, is to connect O-nitroterephthalic acid at the end of the PEG. The stationary phase has weak acidity, suitable for separating neutral and acidic compounds, and the thermal stability of the stationary phase can be increased to  $250\text{ }^{\circ}\text{C}$ .

The selectivity and polarity of stationary phase should be considered, because selectivity is the ability of a stationary phase to distinguish between two component properties (chemical or physical), while polarity depends on the structure of the stationary phase. The selectivity is shown in the following Figure and Table 5.1, and the polarity is shown in Table 5.2.

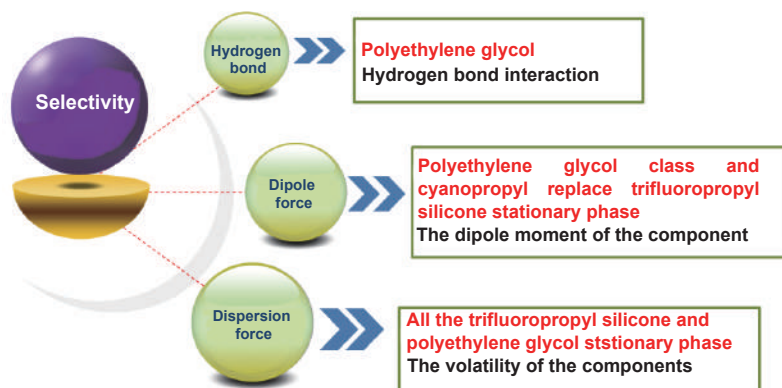

Tab 5.1 Selectivity of stationary phase

| Functional group      | Dispersion force | Dipole force | Hydrogen bond |
|-----------------------|------------------|--------------|---------------|
| Methyl group          | Strong           | No           | No            |
| Phenyl group          | Strong           | No or weak   | Weak          |
| Cyanopropyl           | Strong           | Very strong  | Medium        |
| Propyl three fluorine | Strong           | Medium       | Weak          |
| Polyethylene glycol   | Strong           | Strong       | Medium        |

**Tab 5.2 Polarity of stationary phase**

| Nonpolar |        |        |          | Moderate polarity |          |         | Strong polarity |
|----------|--------|--------|----------|-------------------|----------|---------|-----------------|
| WEL-1    | WEL-5  | WEL-35 | WEL-17   | WEL-1301          | WEL-1701 | WEL-225 | WEL-WAX         |
| WEL-101  | WEL-52 | WM-35  | WEL-XE60 | WEL-624           | WM-1701  | WM-225  | WEL-PEG 20M     |
| WEL-30   | WEL-54 |        | WM-17    | WM-1301           |          | WEL-930 | WEL-INOWAX      |
| WM-1     | WM-5   |        |          | WM-624            |          |         | WEL-FFAP        |
| WM-1MS   | WM-5MS |        |          |                   |          |         | WM-INOWAX       |
| WEL-PONA |        |        |          |                   |          |         | WM-FFAP         |

**Summary of Stationary Phase Selection:**

- (1) Non-polar stationary phase has a longer lifetime than polar stationary phase. If the resolution and analysis time meet the requirements, choose the stationary phase with small polarity as far as possible.
- (2) Usually a stationary phase whose polarity is similar to the component will be chosen, but polarity is only one of the factors affecting separation.
- (3) If you do not know which stationary phase to choose and have no information to refer to, you can start testing from WEL-1 or WEL-5.

**5.1.2 The inner diameter of the column**

The inner diameter of column is an important factor affecting column efficiency, retention, column pressure and column capacity.

Column efficiency (N/m) is inversely proportional to the inner diameter of the column. The resolution is the square root function of the column effect. In theory, the resolution increases to 1.41 times, the column efficiency will be doubled. Therefore, to achieve high column efficiency and separation, we need to use the column with smaller diameter.

At constant temperature, the smaller the inner diameter of the column, the smaller the retention of the component.

The column head pressure is sensitive to the change of column inner diameter, which is about the negative quadratic function of column inner diameter. With the decrease of the inner diameter of the column, the column head pressure increases sharply.

In general, as the diameter of column increases, the capacity of column will increase. The typical column capacity of various columns is shown in Table 5.3.

**Tab 5.3 Column capacity (ng)**

| Film thickness (µm) | Column inner diameter (mm) |           |           |           |
|---------------------|----------------------------|-----------|-----------|-----------|
|                     | 0.18-0.20                  | 0.25      | 0.32      | 0.53      |
| 0.10                | 20-35                      | 25-50     | 35-75     | 50-100    |
| 0.25                | 35-75                      | 50-100    | 75-125    | 100-250   |
| 0.50                | 75-150                     | 100-200   | 125-250   | 250-500   |
| 1.00                | 150-250                    | 200-300   | 250-500   | 500-1000  |
| 3.00                |                            | 400-600   | 500-800   | 1000-2000 |
| 5.00                |                            | 1000-1500 | 1200-2000 | 2000-3000 |

**Summary of Column Inner Diameter Selection:**

- (1) Column with inner diameter of 0.18-0.25mm has high column efficiency. The column with smaller inner diameter has smaller column capacity and larger column head pressure.
- (2) Column with inner diameter of 0.32 mm has large sample capacity. For large volume injection or earlier outflow of components of splitless injection, it has better degree of separation.
- (3) A column of 0.45 mm inner diameter is especially suitable for high carrier gas flow rate, such as sweep traps, headspace injectors and valve injection applications.
- (4) A column of 0.53 mm inner diameter, which is suitable for the situation where equipped with a large-caliber direct sampler. It integrates advantages of sample capacity, column efficiency and injection on the needle, and is increasingly replacing the packing column.

### 5.1.3 Selection of Column Length

Column efficiency (N/m) is proportional to column length. The resolution is the square root function of the column efficiency. Theoretically, if the column length is doubled, the resolution will increase to 1.41 times. However, with the increase of column length and the extension of analysis time, the loss of column will also increase. The cost of column is doubled with the doubling of column length, so increasing column length is the last consideration when increasing column efficiency.

- (1) 25-30 m columns are more commonly used and generally available.
- (2) 10-15m column, especially suitable for the separation of samples containing fewer or easily separated components.
- (3) 50-60m column, suitable for the separation of complex samples containing multiple components.

### 5.1.4 Selection of Column Thickness

- (1) For columns with inner diameter of 0.18-0.32mm and film thickness of 0.18-0.25 $\mu$ m, suitable for most analyses.
- (2) For columns with inner diameter of 0.45-0.53mm and film thickness of 0.8-1.5 $\mu$ m, suitable for most analyses.
- (3) Thick film column is suitable for separation of volatile components.
- (4) Thin film column is suitable for the analysis of components with high molecular weight and high boiling point.

## 5.2 Installation of Capillary Column

The installation of column directly affects the analysis effect and the lifetime of column, so it is crucial to connect column with injection inlet and detector accurately. Installation steps of capillary column are as follows:

#### (1) Preparations before installing

Check the carrier gas and gas filter to ensure the use of auxiliary gas and detector gas; check whether the column is damaged or broken; check the inlet, clean or replace the injection pad and the injection port liner.

#### (2) Cutting columns

Install the nut and card sleeve at one end of the capillary column, and then cut the capillary column port flat.

**Cut capillary column:** first use your finger to support the cutting part of the capillary column, mark the outer wall of the capillary with the corresponding cutting tool. Then hold the column body at 1-2 cm with both hands, pull out and bend the column body. Finally, use a magnifying glass to ensure that the cut port and wall are at right angles without edges or residual debris.

#### (3) Connect the column to the inlet

Generally, the top of the column should be located in the middle and lower part of the inlet liner. Ideally, the distance between the tip of the needle and the top of column is 1-2 cm. When the injection needle passes through the spacer to insert the injection port.

**Installation of connecting nut:** after the column is embedded in the injection port, the connecting nut is screwed by hand, and when the hand is not twisted, the wrench 1/4-1/2 is used to ensure the sealing of the installation.

#### (4) Gas connection

After the column and the inlet are connected, the carrier gas should be connected, and then the suitable carrier gas flow rate can be obtained by adjusting the pre-pressure of the column. The relationship among column front pressure and column length and column inner diameter is shown in Table 5.4.

**Tab 5.4 Similar column pre-pressure(Psig)**

| Column length (m) | Inner diameter (mm) |       |      |
|-------------------|---------------------|-------|------|
|                   | 0.25                | 0.32  | 0.53 |
| 15                | 8-12                | 5-10  | 1-2  |
| 20/30             | 15-25               | 10-20 | 2-4  |

| Column length (m) | Inner diameter (mm) |       |      |
|-------------------|---------------------|-------|------|
|                   | 0.25                | 0.32  | 0.53 |
| 50/60             | 30-45               | 20-30 | 4-8  |
| 75                |                     |       | 5-10 |
| 105               |                     |       | 7-15 |

Insert the other end of the column into the sample vial containing hexane. After the carrier gas is connected, the stable and continuous foaming appears in the bottle, indicating that the connection is normal, otherwise, the carrier gas device and flow should be rechecked.

Quantity control device and air tightness. After the problem is solved, take the column from the sample vial, wipe inlet without solvent residue, prepare for the next installation.

**Precaution:** hydrogen as carrier gas, be sure to pay attention to safety. When the content of hydrogen in the air reaches 4%-10%, there is a risk of explosion, and diffusion of gas needs to speed up.

(5) Column connected to detector

The connection between column and detector is almost the same as step (3).

**Precaution:** when the detector is ECD or NPD, in order to enable the detector to achieve stability in a shorter time, do not connect it to the detector when aging column.

(6) Gas leak detection

The GC system must be detected before heating column. Electronic leak detector is one of the most convenient and fastest methods for carrier gas leak detection of inlet and detector.

**Precaution:** the inlet and detector for carrier gas leak detection, do not to use Snoop and other soap bubbles to avoid pollution or damage to the system.

(7) Determination of carrier gas flow and inspection of column installation

After installing the column, adjust the carrier gas flow rate or the sample chromatogram of the non-reserved compound is analyzed to verify the correct installation of the injection port and detector. Common non-reserved compounds are shown in Table 5.5.

**Tab 5.5 Common non-retention compounds(Psig)**

| Detector | Compound                        |
|----------|---------------------------------|
| FID      | Methane, butane                 |
| TCD      | Methane, butane, argon, air     |
| ECD      | Methylene chloride, SF6, CF2Cl2 |
| NPD      | Acetonitrile                    |
| PID      | acetylene, ethylene             |
| MS       | Methane, butane, argon, air     |

(8) Aging and test of columns

If the temperature of the column oven is set to the maximum operating temperature, or 20 °C above the maximum analytical temperature (whichever is lower), the column is aged for 2-3 hours under that temperature.

Under normal circumstances, in the initial stage, the baseline shows a continuous upward trend. After reaching the aging temperature for 5-10 min, the baseline begins to decline and last about 30-90 min, finally, baseline stabilizes.

Confirm the flow rate of carrier gas by testing the sample of non-retention substance again.

## 5.3 Troubleshooting of GC column

### 5.3.1 Reasons for Declination of GC Column Properties

## (1) Fracture of column

For the GC capillary column, the polyimide coating can protect the elastic fused quartz tube, and the column rarely breaks naturally. Attention should be paid to avoid the label of column, metal edge in column oven and other articles with sharp edge scratching polyimide coating, resulting in the phenomenon of column fracture. Moreover, the 0.45-0.53 mm column tube is more prone to fracture than the inner diameter 0.18-0.32 mm column tube.

## (2) Heat damage

When the analytical temperature is higher than the maximum operating temperature, the stationary phase and the inner surface of the column tube will be damaged, resulting in the loss of the column, the decline of the column efficiency and the deterioration of the peak type. Thermal damage is a slow process, only if column operates upper limit is temperature for a long time, will obvious damage occur. However, in the presence of high concentration of oxygen, the overheating of the column will cause rapid and permanent damage to the column.

It is suggested that the maximum temperature of the column oven should be set as the upper temperature limit of the column or slightly lower than the upper temperature limit to avoid accidental overheating of the column. If the column is hot damaged, the detector end can be cut off about 10 cm. Even aging or having column efficiency test, the column can not completely restore to the original performance, but it may still work. The column lifetime after thermal damage will be shortened.

## (3) Oxygen damage

For most capillary columns, oxygen is a nuisance. Under the condition of oxygen, the stationary phase degrades rapidly with the increase of column temperature, resulting in column loss, column efficiency decrease and peak type variation. Compared with the thermal damage of the column, the column has been seriously damaged when oxygen damage is found. Especially for polar capillary column, the temperature and oxygen concentration which can cause serious damage to column are very low.

Continuous contact with oxygen will cause oxygen damage, short contact with oxygen, such as a single air injection will not be a problem.

The purity of carrier gas or the leakage of carrier gas flow path is the source of oxygen exposure, so keeping the system oxygen free and leakage free is the best choice to prevent the oxygen damage of column. It is recommended to have gas leak detection regularly, to use high purity carrier gas, and to replace oxygen capture hydrazine and gas cylinders timely.

## (4) Chemical damage

The compounds that produce chemical damage to the column are mainly inorganic or mineral acids and mineral bases. Acids include hydrochloric acid (HCl), sulfuric acid (H<sub>2</sub>SO<sub>4</sub>), nitric acid (HNO<sub>3</sub>), phosphoric acid (H<sub>3</sub>PO<sub>4</sub>) and chromic acid (CrO<sub>3</sub>). Bases include potassium hydroxide (KOH), sodium hydroxide (NaOH) and ammonium hydroxide (NH<sub>4</sub>OH). They are less volatile, easy to remain at the front of the column. If you don't clear them in time, they will damage the stationary phase, resulting in column loss, reduced column efficiency and poor peak type. Among them, hydrochloric acid and ammonium hydroxide do least damage to stationary phase. The damage of the two substances to the column is often accompanied by the existence of water. These two kinds of damage often occur with the water in the sample. The retention time of HCl and NH<sub>4</sub>OH in the column will be very short and the damage to the column will be weakened if the column has little or no retention of water under certain conditions.

Only compounds such as perfluorinated acids, including trifluoroacetic acid, pentafluoropropionic acid and heptafluorobutyric acid, have been reported to produce chemical damage to columns. A concentration of 1% or more of these substances can damage the stationary phase of the column. Most of the problems occur in direct injection of non-shunt or large diameter columns.

Chemical damage is often limited to the front end of the column, cut off the front end of the column of 0.5-1 m and eliminate chromatographic problems. In more serious cases, it may be necessary to intercept longer columns. Using pre-columns or retaining gap tubes can minimize chemical damage to columns, but regular replacement of pre-columns is required.

## (5) Contaminated column

Column contamination is also a common problem in gas phase analysis. The pollutants in the column are divided into two categories: non-volatile and semi-volatile. The nonvolatile remains in the column and is distributed on the inner surface of the column, affecting the distribution of the components in the stationary phase. In addition, the nonvolatile also interacts with the active components (compounds containing hydroxyl, amino, mercapto or aldehyde groups), resulting in the-type tailing of the active components and the decrease of the responder. Then semi-volatile contaminants will accumulate in the chromatography, causing peak type, response intensity, and baseline

There are many sources of column pollution, and samples are the most common and direct source. Such as biological fluids, soil, wastewater and groundwater, all contain large amounts of nonvolatile and semi-volatile components. The semi-volatile and non-volatile components in the sample are more easily accumulated in the column, resulting in column contamination.

Complete sample purification is the best way to prevent contamination, and the use of protective or protective clearance tubes can reduce the degree of contamination.

## 5.3.2 Troubleshooting

### Problem 1: Tailing area and solutions

1. Injector liner pollution: clean liner, or remove 1~2 laps of the column inlet to use.
2. Temperature of column or injector temperature is too low: rise temperature (do not exceed maximum temperature).
3. Overload caused by the too large injection volume: adjust the tailing blowing flow and split ratio.
4. Co-elution of two compounds: reduce the rate of rising column temperature and increase the resolution. Improve the sensitivity and reduce the injection volume.
5. Column damage: replace column
6. Column pollution: remove 1~2 laps from the inlet end of the column and reinstall; if it does not work, aging columns is required; furthermore, the clean column with solvent, but this method is only suitable for bonded crosslinked stationary phase.
7. Mismatch of solvent phase and polarity : earlier outflow peaks or peaks near the solvent front are more likely to tail and change the sample solvent.

### Problem 2: Leading area and solutions

1. Overload caused by injection volume: reduce sample injection volume.
2. Co-elution of two compounds: reduce the rate of rising column temperature and increase the resolution. Improve the sensitivity and reduce the injection volume.
3. Sample decomposition: reduce the inlet temperature and use deactivated liner.
4. Sample condensation: if necessary, increase the inlet temperature and column temperature.

### Problem 3: No peak and solution

1. Injection needle leakage or blockage: clean or replace injection needle.
2. leakage of Injection pad: replace injection pad.
3. Inlet temperature is too low: increase the inlet temperature to ensure the complete gasification of the sample.
4. Column temperature is too low: rise column temperature, avoid sample condensation in column.
5. When injecting automatically, the sample quantity in the sample is insufficient, the sample needle can not absorb the sample: normally, the sample quantity should be 0.8-1.2ml.
6. Blockage or leakage at the connection between the column and the inlet, the column and the detector: leak detection and reinstall if necessary.
7. If FID detector was used the flame may be extinguished or the polarization voltage is not added: check and re-ignite.
8. Recorder line connection or damage: check the line or replace the recorder.
4. Detector leakage: check leakage
5. Injector pad degradation: change sample pad

### Problem 4: Baseline instability and solutions

1. Carrier gas deficiency: check carrier gas pressure, if less than 500 psi, timely replace gas cylinders
2. Gas purity is not enough or gas path pollution: replace gas cylinders or use gas purification devices
3. The flow rate of carrier gas is not within the limit of the instrument: measure the flow rate and adjust it according to the instrument manual.
4. sampler or detector contamination: cleaning
5. Injection pad leakage: replace injection pad
6. liner pollution: cleaning liner, replace quartz cotton;
7. Column loss or contamination: replace liner; or cut off 1-2 laps at the inlet end of column; or aging treatment.

### Problem 5: Excessive baseline noise and solutions

1. Injector or detector contamination: clean injector, replace liner and injection pad; clean detector;
2. Carrier gas purity is not enough or pollution: use high purity gas; check gas purifier for expiration or leakage;
3. Carrier gas flow rate is not suitable: adjust the gas flow rate to the recommended value;

4. Detector leakage: check leakage
5. Injector pad degradation: change sample pad.
6. liner pollution: cleaning liner, replace quartz cotton;
7. Column loss or contamination: replace liner or cut off 1-2 laps at the inlet end of column. Through aging treatment.

### Problem 6: Peak broadening and solutions

1. Injection technology: rapid and stable injection technology
2. Carrier gas flow rate: adopt recommended carrier gas flow rate
3. Sample concentration: reduce sample concentration
4. Sample solvent effect: when using ECD detector, you can not use dichloromethane and other solvents.
5. Column contaminated: cut the front end of the column 1-2 laps.

### Problem 7: Retention time fluctuations and solutions

1. Carrier gas flow rate change: check carrier gas flow rate;
2. Column temperature change: check column temperature;
3. Column specification change: check column specification model consistency;
4. Injector leakage: leak detection;
5. Injection spacer leakage: replace spacer;
6. Gas path blockage: cleaning or replacing gas pipeline.

### Problem 8: Split peaks and solutions

1. Mixed sample solvent: change the sample solvent to a single solvent;
2. Column incorrect installation: reinstall column;
3. Injection needle contamination: clean injection needle;
4. Sample degradation in injector: reduce injector temperature, and ensure sample gasification but can not decompose.


## 5.3.3 Troubleshooting Case Analysis

General troubleshooting requires several steps: identify problems, collect information, think about plans, test, repair, and record.


### 1. Ghost Peaks

(1) Confirm question:

Abnormal Chromatogram

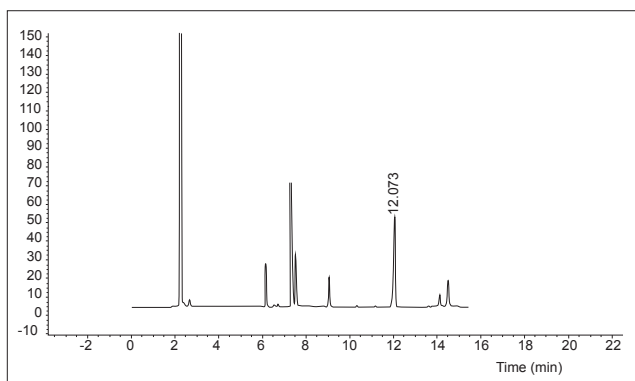

Referring Chromatogram

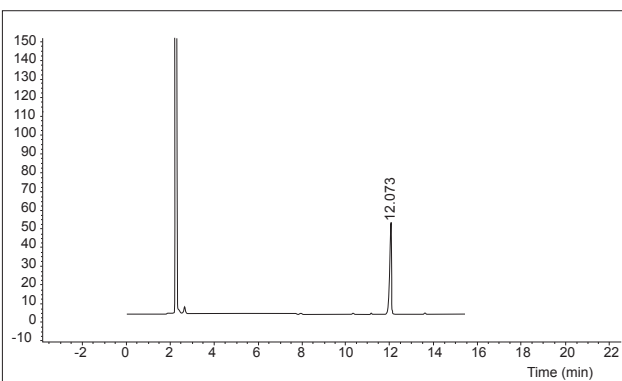

- ✗ With ghost peaks
- ✗ The results of the second of injection are the same

(2) Collect information

- EPC system, Manual injection, S/SLinlet, FID
- All the operational parameters are correct
- Without other phenomena
- Using the same gas source and column to do the same batch of samples with another GAS FID has no problem
- Device has not maintained recently



### (3) Think plans



Possible sources of ghost peaks: sample, solvent, injection needle, gas cylinder, gas purification pipe, gas pipeline, inlet, column, detector.

Using another GC FID but the same column to do the same batch of samples has no problem, exclude the problems of solvent, samples, gas cylinders, gas purification pipe, gas pipeline, column problems.


Contamination of injection needle, injection port and detector should be further checked in the following experiments.

### (4) Test results

- Empty injection (without injection): have ghost peaks, the pollution is most likely to be changed by temperature shadow solvent blank (only into the solvent) : there is ghost peak, which means that the pollution may be in the area where the solvent goes through the noise -- the injector, the detector.

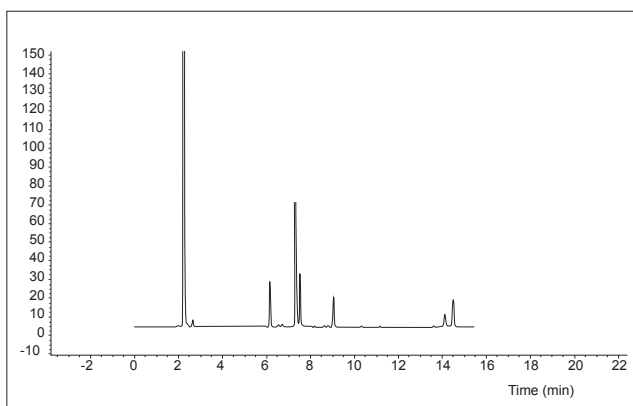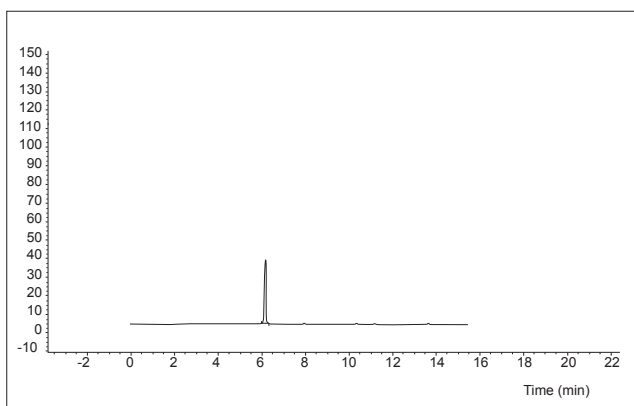

- Replace injection needle and run with empty injection: ghost peak, indicating contamination may be in the area where the solvent passes or the solvent itself, but not from the injection needle - injection inlet, detector

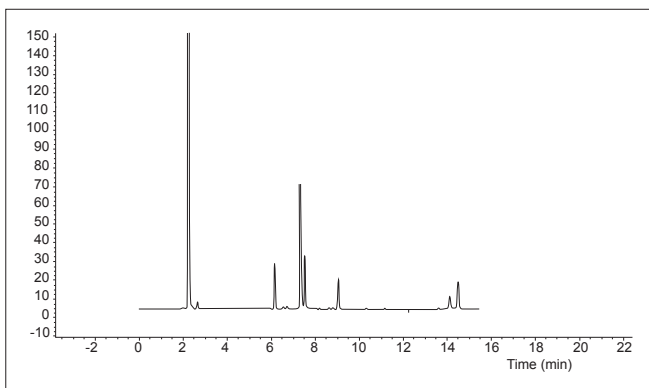




Conclusion: After screening, the remaining two areas are injection inlet and detector

### (5) Repair

- Injection inlet maintenance: replace the injection pad, replace the liner and quartz cotton
- Detector maintenance: cleaning nozzle


### (6) Record

- System performance can be restored to reference conditions

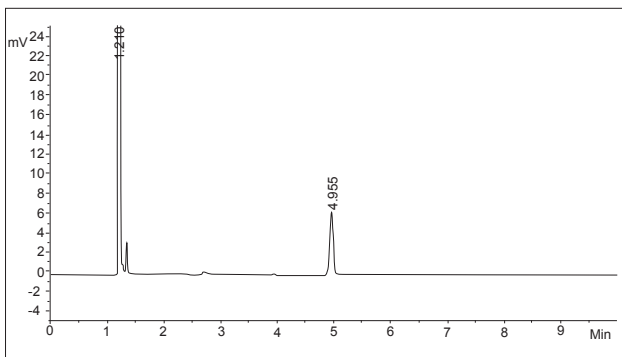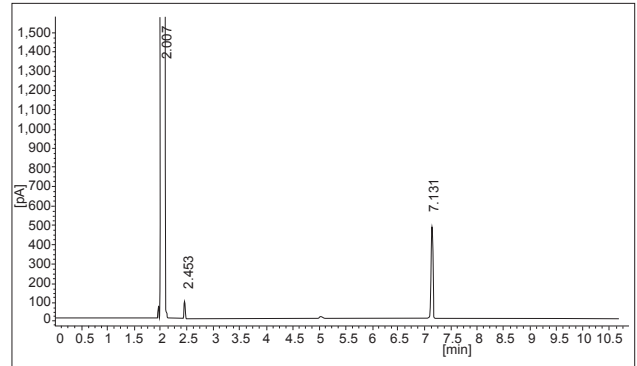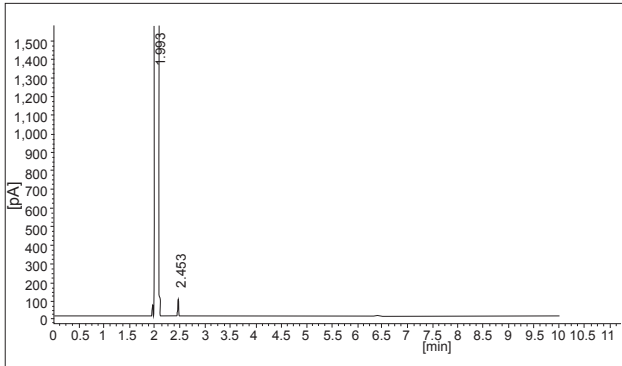


(2) Water as solvent (FID Detector)

Abnormal chromatogram

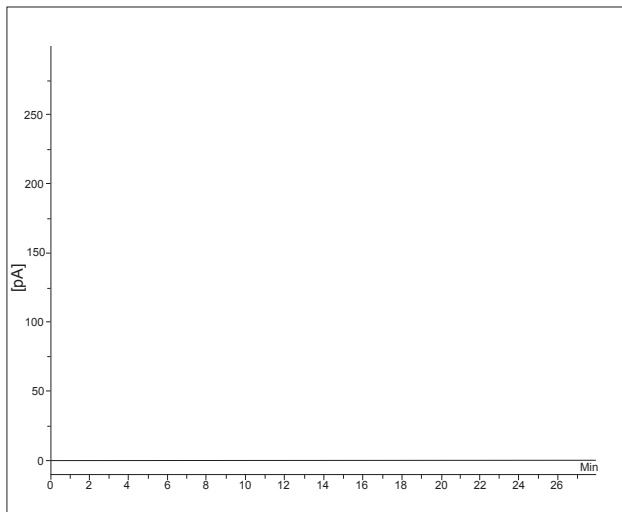


Referring chromatogram

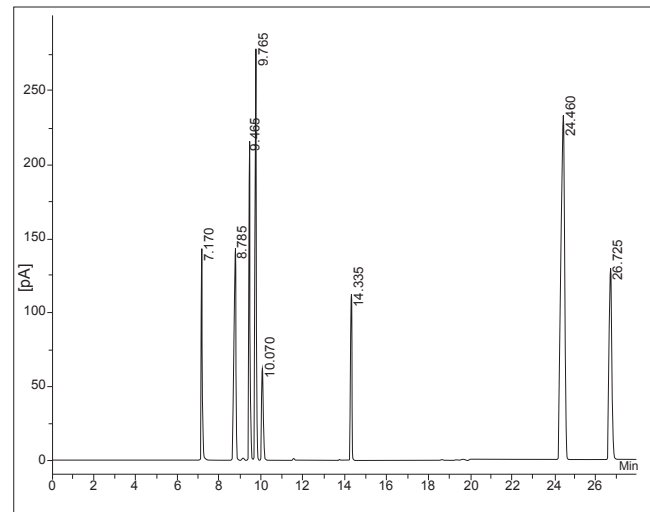


Conclusion: the reason for unappearance of peaks is the sensibility of GC device can't achieve the test requirements

(3) There's no solvent peak

Abnormal chromatogram

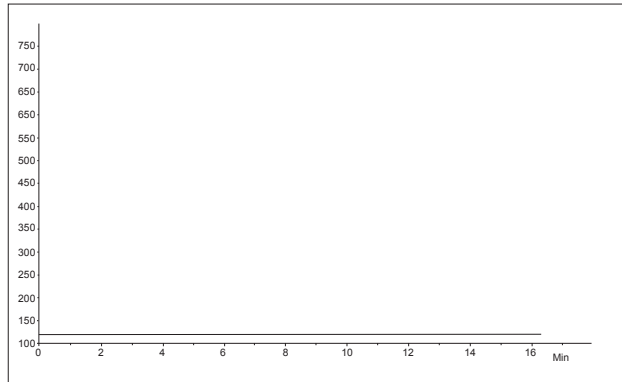

Chromatogram for reinstalling the column

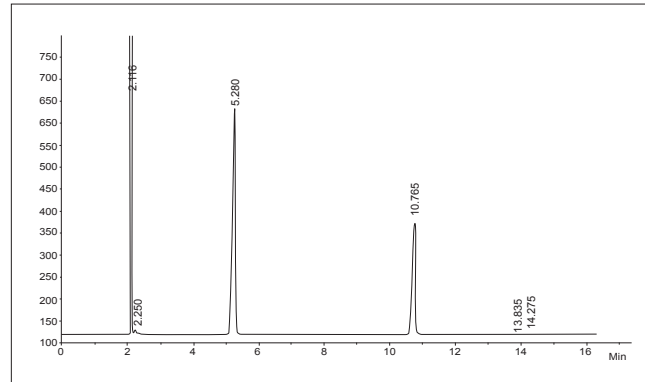

Conclusion: the reason for unappearance of peaks is that the column is not installed accurately or there is air leakage at the connection between the column and the inlet of detector.



Москва, 115230, Каширское шоссе, д. 3, кор. 2, стр. 4/9

+7 (495) 640 4192

+7 (499) 682 6555

[chrom@chimmed.ru](mailto:chrom@chimmed.ru)

[www.chimmed.ru](http://www.chimmed.ru)